

Recommended Practice for Centralizer Placement and Stop-collar Testing

ANSI/API RECOMMENDED PRACTICE 10D-2
FIRST EDITION, AUGUST 2004

REAFFIRMED, APRIL 2015

**ISO 10427-2:2004 (Identical), Petroleum and natural gas industries—Equipment for well cementing—
Part 2: Centralizer placement and stop-collar testing**



AMERICAN PETROLEUM INSTITUTE



Special Notes

API publications necessarily address problems of a general nature. With respect to particular circumstances, local, state, and federal laws and regulations should be reviewed.

API is not undertaking to meet the duties of employers, manufacturers, or suppliers to warn and properly train and equip their employees, and others exposed, concerning health and safety risks and precautions, nor undertaking their obligations under local, state, or federal laws.

Information concerning safety and health risks and proper precautions with respect to particular materials and conditions should be obtained from the employer, the manufacturer or supplier of that material, or the material safety data sheet.

Nothing contained in any API publication is to be construed as granting any right, by implication or otherwise, for the manufacture, sale, or use of any method, apparatus, or product covered by letters patent. Neither should anything contained in the publication be construed as insuring anyone against liability for infringement of letters patent.

Generally, API standards are reviewed and revised, reaffirmed, or withdrawn at least every five years. Sometimes a one-time extension of up to two years will be added to this review cycle. This publication will no longer be in effect five years after its publication date as an operative API standard or, where an extension has been granted, upon republication. Status of the publication can be ascertained from the API Standards department telephone (202) 682-8000. A catalog of API publications, programs and services is published annually and updated biannually by API, and available through Global Engineering Documents, 15 Inverness Way East, M/S C303B, Englewood, CO 80112-5776.

This document was produced under API standardization procedures that ensure appropriate notification and participation in the developmental process and is designated as an API standard. Questions concerning the interpretation of the content of this standard or comments and questions concerning the procedures under which this standard was developed should be directed in writing to the Director of the Standards department, American Petroleum Institute, 1220 L Street, N.W., Washington, D.C. 20005. Requests for permission to reproduce or translate all or any part of the material published herein should be addressed to the Director, Business Services.

API standards are published to facilitate the broad availability of proven, sound engineering and operating practices. These standards are not intended to obviate the need for applying sound engineering judgment regarding when and where these standards should be utilized. The formulation and publication of API standards is not intended in any way to inhibit anyone from using any other practices.

Any manufacturer marking equipment or materials in conformance with the marking requirements of an API standard is solely responsible for complying with all the applicable requirements of that standard. API does not represent, warrant, or guarantee that such products do in fact conform to the applicable API standard.

These materials are subject to copyright claims of ISO, ANSI and API.
All rights reserved. No part of this work may be reproduced, stored in a retrieval system, or transmitted by any means, electronic, mechanical, photocopying, recording, or otherwise, without prior written permission from the publisher. Contact the Publisher, API Publishing Services, 1220 L Street, N.W., Washington, D.C. 20005.

Copyright © 2004 American Petroleum Institute

API Foreword

This standard shall become effective on the date printed on the cover but may be used voluntarily from the date of distribution.

API publications may be used by anyone desiring to do so. Every effort has been made by the Institute to assure the accuracy and reliability of the data contained in them; however, the Institute makes no representation, warranty, or guarantee in connection with this publication and hereby expressly disclaims any liability or responsibility for loss or damage resulting from its use or for the violation of any federal, state, or municipal regulation with which this publication may conflict.

Standards referenced herein may be replaced by other international or national standards that can be shown to meet or exceed the requirements of the referenced standard.

Suggested revisions are invited and should be submitted to the API, Standards Department, 1220 L Street, NW, Washington, DC 20005, or by email to standards@api.org.

The form in this annex is intended for free exchange between owners/operators of the equipment or users of API RP 10D-2.

This American National Standard is under the jurisdiction of the API Subcommittee on Well Cements, SC10. This standard is considered identical to the English version of ISO 10427-2. ISO 10427-2 was prepared by Technical Committee ISO/TC 67 Materials, equipment and offshore structures for petroleum and natural gas industries, SC 3 Drilling and completion fluids, and well cements.

Contents

	Page
API Foreword	ii
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Methods for estimating centralizer placement	3
4.1 General	3
4.2 Standoff ratio calculation	4
4.3 Buoyed weight of casing	5
4.4 Calculations for centralizer spacing	6
5 Procedure for testing stop collars	9
5.1 General	9
5.2 Apparatus	10
5.3 Test procedure	11
5.4 Reporting of test results	11
Annex A (informative) Documentation of stop-collar test results	12
Bibliography	14

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 10427-2 was prepared by Technical Committee ISO/TC 67, *Materials, equipment and offshore structures for petroleum, petrochemical and natural gas industries*, Subcommittee SC 3, *Drilling and completion fluids, and well cements*.

This first edition of ISO 10427-2, together with ISO 10427-1 and ISO 10427-3, cancels and replaces ISO 10427:1993, which has been technically revised.

ISO 10427 consists of the following parts, under the general title *Petroleum and natural gas industries — Equipment for well cementing*:

- *Part 1: Casing bow-spring centralizers*
- *Part 2: Centralizer placement and stop-collar testing*
- *Part 3: Performance testing of cementing float equipment*

Introduction

This part of ISO 10427 is based on API Specification 10D, 5th edition, January 1995^[1].

In this part of ISO 10427, where practical, U.S. Customary units are included in brackets for information.

Petroleum and natural gas industries — Equipment for well cementing —

Part 2: Centralizer placement and stop-collar testing

1 Scope

This part of ISO 10427 provides calculations for determining centralizer spacing, based on centralizer performance and desired standoff, in deviated and dogleg holes in wells for the petroleum and natural gas industries. It also provides a procedure for testing stop collars and reporting test results.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 11960, *Petroleum and natural gas industries — Steel pipes for use as casing or tubing for wells*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply:

3.1

annular clearance for perfectly centred casing

wellbore diameter minus casing outside diameter divided by two

3.2

centralizer permanent set

change in centralizer bow height after repeated flexing

NOTE A bow-spring centralizer is considered to have reached permanent set after being flexed 12 times.

3.3

flexed

condition of a bow-spring when a force three times the specified minimum restoring force ($\pm 5\%$) has been applied to it

[ISO 10427-1:2001, 3.1]

NOTE Specified minimum restoring force values are found in Table 1 of ISO 10427-1:2001.

3.4

holding device

device employed to fix the stop collar or centralizer to the casing

EXAMPLE Set screws, nails, mechanical dogs and epoxy resins.

[ISO 10427-1:2001, 3.2]

3.5

holding force

maximum force required to initiate slippage of a stop collar on the casing

[ISO 10427-1:2001, 3.3]

3.6

hole size

diameter of the wellbore

[ISO 10427-1:2001]

3.7

limit clamp

equivalent term for a stop collar

3.8

restoring force

force exerted by a centralizer against the casing to keep it away from the wellbore wall

NOTE Restoring-force values can vary based on the installation methods.

[ISO 10427-1:2001, 3.5]

3.9

rigid centralizer

centralizer manufactured with bows, blades or bars that do not flex

NOTE Adapted from ISO 10427-1:2001, 3.6.

3.10

running force

maximum force required to move a centralizer through a specified wellbore diameter

NOTE Running-force values can vary based on the installation methods.

[ISO 10427-1:2001]

3.11

sag point

point where the casing deflection is at a maximum

NOTE Casing that is supported at two points will tend to sag between the support points, this sag is called the casing sag or casing deflection.

3.12

slippage force range

range of forces required to continue to move a stop collar after the holding force has been overcome

3.13

solid centralizer

centralizer manufactured in such a manner as to be a solid device with nonflexible fins or bands

NOTE These centralizers have solid bodies and solid blades.

3.14

standoff

smallest distance between the outside diameter of the casing and the wellbore

[ISO 10427-1:2001, 3.8]

3.15

standoff ratio

R_s

ratio of standoff to annular clearance for perfectly centred casing

NOTE 1 It is expressed as a percentage.

NOTE 2 Adapted from ISO 10427-1:2001, 3.9.

3.16

starting force

maximum force required to insert a centralizer into a specified wellbore diameter

NOTE Starting-force values can vary based on the installation methods.

[ISO 10427-1:2001, 3.10]

3.17

stop collar

device attached to the casing to prevent movement of a casing centralizer

NOTE A stop collar can be either an independent piece of equipment or integral with the centralizer.

[ISO 10427-1:2001, 3.11]

4 Methods for estimating centralizer placement

4.1 General

The equations presented below are based on certain assumptions and are considered sufficiently accurate for general use. More specific calculations based on complete wellbore data may be available but are beyond the scope of this document.

There is no recommendation or requirement for a specific standoff ratio for casing centralization. The standoff ratio of 67 % is used in the specification for the purpose of setting a minimum standard for performance of casing bow-spring centralizers only. This number is used only in the specifications for bow-spring type centralizers and deals with the minimum force for each size of centralizer at that standoff. The 67 % standoff ratio is not intended to represent the minimum acceptable amount of standoff required to obtain successful centralization of the casing. The user is encouraged to apply the standoff ratio required for specific well conditions based on well requirements and sound engineering judgement.

Even a minor change in inclination and/or azimuth, with the string of casing hanging below it, materially affects the standoff and the requirements for centralizer placement.

The lateral load (force) on a centralizer is composed of two components. The first is the weight component of the section of pipe supported by the centralizer, and the second is the tension component exerted by the pipe hanging below the centralizer.

4.2 Standoff ratio calculation

Annular clearance (l_a) for perfectly centred casing can be calculated as follows (see Figure 1):

$$l_a = \frac{D_w - D_p}{2} \quad (1)$$

where

l_a is the annular clearance for perfectly centred casing, expressed in metres (inches);

D_w is the wellbore diameter, expressed in metres (inches);

D_p is the casing outside diameter, expressed in metres (inches).

The standoff at the centralizer in a given hole size is represented by the symbol S_c (see Figure 1). The standoff at a bow-spring centralizer is taken from the load deflection curve of the centralizer, tested in that hole size, based upon the lateral load applied (see ISO 10427-1:2001, A.1 [2]).

NOTE Differences in hole size alter the load-deflection curve of a centralizer.

Since the bows or blades of a solid or rigid centralizer do not deflect, the standoff at the centralizer is determined using the rigid or solid blade diameter as follows:

$$S_c = \frac{D_c - D_p}{2} \quad (2)$$

where

S_c is the standoff at the centralizer, expressed in metres (inches);

D_c is the outside diameter of the centralizer solid or rigid blades, expressed in metres (inches).

Standoff at the sag point may be determined by Equation (3), which considers the deflection of the casing string and compression of the centralizers due to lateral load (Figure 1).

$$S_s = S_c - \delta \quad (3)$$

where

S_s is the standoff at the sag point, expressed in metres (inches);

δ is the maximum deflection of the casing between centralizers, expressed in metres (inches).

The minimum standoff may occur at the location between centralizers where the deflection (δ) of the casing is at its maximum or at the centralizers. Therefore, standoff (S) of a section of casing is the minimum value of standoff at the centralizers (S_c) or standoff at the sag point (S_s).

The standoff ratio (R_s) may be calculated as follows:


$$R_s = \frac{S}{l_a} \times 100 \quad (4)$$

where

R_s is the standoff ratio, expressed as a percentage;

S is the standoff, expressed in metres (inches);

l_a is the annular clearance for perfectly centred casing, expressed in metres (inches).

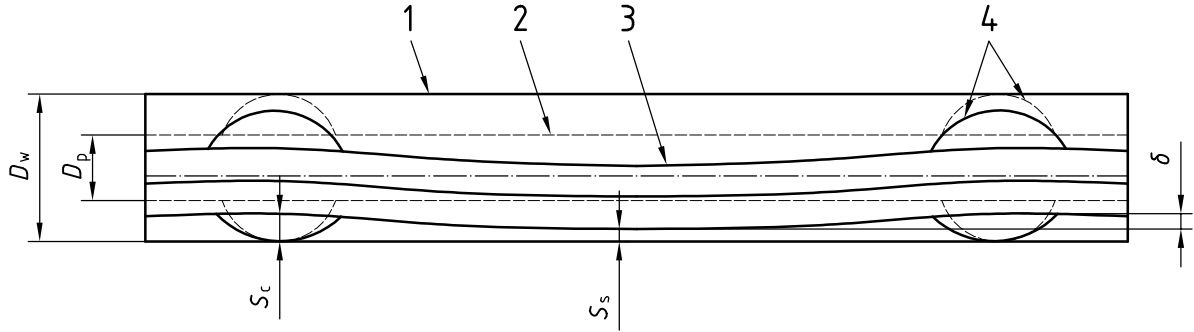

Key

- | | |
|------------------------------|------------------------------------|
| 1 wellbore | δ maximum casing deflection |
| 2 casing (perfectly centred) | D_p casing outside diameter |
| 3 casing (deflected) | D_w wellbore diameter |
| 4 centralizer | S_c standoff at the centralizer |
| | S_s standoff at the sag point |

Figure 1 — Calculation of casing standoff in a wellbore

4.3 Buoyed weight of casing

4.3.1 General

The buoyed weight of casing is the effective weight of the casing in the well. Consideration is given to the densities of the fluids inside and outside the casing, and the weight of the casing in air.

4.3.2 Generalized equation

The following is a generalization of the treatment of effective weight of casing to accommodate different internal and external fluids, based upon a model developed by Juvkam-Wold and Baxter [3].

$$W_b = W \cdot f_b \quad (5)$$

$$f_b = \frac{\left(1 - \frac{\rho_e}{\rho_s}\right) - \left(\frac{D_i}{D_p}\right)^2 \left(1 - \frac{\rho_i}{\rho_s}\right)}{\left(1 - \frac{D_i^2}{D_p^2}\right)} \quad (6)$$

where

W_b is the unit buoyed weight of the casing, expressed in newtons per metre (pound-force per inch);

W is the unit weight of casing in air, expressed in newtons per metre (pound-force per inch);

f_b is the buoyancy factor;

D_i is the inside diameter of the casing, expressed in metres (inches);

D_o is the casing outside diameter, expressed in metres (inches);

ρ_i is the density of the fluid inside the casing, expressed in kilograms per cubic metre (pound-mass per gallon);

ρ_s is the density of the casing, expressed in kilograms per cubic metre (pound-mass per gallon);

ρ_e is the density of the fluid outside the casing, expressed in kilograms per cubic metre (pound-mass per gallon).

4.3.3 Discussion

The buoyed weight of the casing being cemented changes during a cementing operation. As the densities of the fluids inside the casing and the annulus change, the relative buoyed weight tends to reach a maximum when the highest density fluid is inside the casing, and a minimum when the highest density fluid is in the annulus. In the calculation of buoyed weight for centralizer spacing, the densities of the fluids both inside the casing and in the annulus should be considered. The calculated centralizer spacing can vary depending on the selection of fluid densities present during the cement job. The standoff ratio will change as the fluid densities change, and the user should note at what point during the cement job the required centralization standoff ratio needs to be met, and the appropriate buoyed weight for use in the calculations.

4.4 Calculations for centralizer spacing

4.4.1 General

The equations are valid only for casing strings with axial tension and do not apply for casing strings under compression. The equations do not consider end effects, for example at the shoe, the wellhead, or the liner hanger. The equations are valid only for calculating the casing deflection between two identical centralizers. The lateral load calculations are based upon a “soft string model” and do not take into effect casing stiffness. Additional models have been developed that consider the effects of compression on the casing standoff and lateral loads [4].

4.4.2 Casing deflection in a one-dimensional (1-D) straight, inclined wellbore without axial tension

In an inclined wellbore with no doglegs and negligible axial tension or compression in the casing, the casing deflection at the sag point between two centralizers can be calculated as follows:

$$\delta = \frac{(W_b \cdot \sin \theta) l_c^4}{384 E \cdot I} \quad (7)$$

where

δ is the maximum deflection of the casing between centralizers, expressed in metres (inches);

W_b is the unit buoyed weight of the casing, expressed in newtons per metre (pound-force per inch);

θ is the wellbore inclination angle, expressed in degrees;

l_c is the distance between centralizers, expressed in metres (inches);

E is the modulus of elasticity of the casing, expressed in newtons per square metre (or pascals) (pound-force per square inch);

I is the moment of inertia of the casing, expressed in m^4 (in^4).

The lateral load of a length (l_c) of casing can be calculated as follows:

$$F_l = W_b \cdot l_c \cdot \sin \theta \quad (8)$$

where F_l is the lateral load, expressed in newtons (pound-force).

4.4.3 Casing deflection in a 1-D straight, inclined wellbore with axial tension

Equation (9) incorporates the effects of tension and can be used to determine the maximum casing deflection in a wellbore that is inclined, but has no doglegs or changes in direction.

$$\delta = \left(\frac{(W_b \cdot \sin \theta) l_c^4}{384 E \cdot I} \right) \left(\frac{24}{\mu^4} \right) \left(\frac{\mu^2}{2} - \frac{\mu \cdot \cosh \mu - \mu}{\sinh \mu} \right) \quad (9)$$

$$\mu = \sqrt{\frac{F_t \cdot l_c^2}{4 E \cdot I}} \quad (10)$$

where F_t is the effective tension below the centralizer, expressed in newtons (pound-force).

4.4.4 Casing deflection in a 2-D wellbore

Casing deflection in a two-dimensional wellbore section that has a constant curvature in a vertical plane can be calculated by the following expressions:

$$\delta = \left[\frac{\left(W_b \cdot \sin \bar{\theta} + \frac{F_t}{r} \right) l_c^4}{384 E \cdot I} \right] \left(\frac{24}{\mu^4} \right) \left(\frac{\mu^2}{2} - \frac{\mu \cdot \cosh \mu - \mu}{\sinh \mu} \right) \quad (11)$$

where

$\bar{\theta}$ is the average wellbore inclination between two centralizers, expressed in degrees;

r is the radius of curvature of the wellbore path, expressed in metres (inches).

or

$$\delta = \left(\frac{F_l \cdot l_c^3}{384 E \cdot I} \right) \left(\frac{24}{\mu^4} \right) \left(\frac{\mu^2}{2} - \frac{\mu \cdot \cosh \mu - \mu}{\sinh \mu} \right) \quad (12)$$

In a 2-D wellbore with decreasing inclination, the lateral load can be expressed as:

$$F_l = W_b \cdot l_c \cdot \sin \bar{\theta} + 2F_t \cdot \sin \frac{\beta}{2} \quad (13)$$

where β is the total angle change between centralizers, expressed in degrees.

In a 2-D wellbore with increasing inclination, the lateral load can be expressed as:

$$F_l = W_b \cdot l_c \cdot \sin \bar{\theta} - 2F_t \cdot \sin \frac{\beta}{2} \quad (14)$$

4.4.5 Casing deflection in a 3-D wellbore

Casing deflection in wellbores with changes in inclination and azimuth can be calculated using the following formulae derived by Juvkam-Wold and Wu [5]. Equation (15) is used to calculate the lateral load of a length of casing (l_c) in the dogleg plane for a drop-off wellbore where the inclination decreases with increasing measured depth. Equation (16) is used to calculate the lateral load of a length of casing (l_c) in a build-up wellbore where the inclination increases with increasing measured depth.

$$F_{l,dp} = W_b \cdot l_c \cdot \cos \gamma_n + 2F_t \cdot \sin \frac{\beta}{2}, \text{ or} \quad (15)$$

$$F_{l,dp} = W_b \cdot l_c \cdot \cos \gamma_n - 2F_t \cdot \sin \frac{\beta}{2} \quad (16)$$

$$\cos \gamma_n = \frac{\sin[(\theta_1 - \theta_2)/2]}{\sin(\beta/2)} \sin\left(\frac{\theta_1 + \theta_2}{2}\right) \quad (17)$$

$$\beta = \cos^{-1}[\cos \theta_1 \cos \theta_2 + \sin \theta_1 \sin \theta_2 \cos(\phi_2 - \phi_1)] \quad (18)$$

$$F_{l,p} = W_b \cdot l_c \cdot \cos \gamma_0 \quad (19)$$

$$\cos \gamma_0 = \frac{\sin \theta_1 \sin \theta_2 \sin(\phi_2 - \phi_1)}{\sin \beta} \quad (20)$$

$$\delta = \left(\frac{F_l \cdot l_c^3}{384 E \cdot I} \right) \left(\frac{24}{\mu^4} \right) \left(\frac{\mu^2}{2} - \frac{\mu \cdot \cosh \mu - \mu}{\sinh \mu} \right) \quad (21)$$

$$F_l = \sqrt{F_{l,dp}^2 + F_{l,p}^2} \quad (22)$$

where

γ_n is the angle between the gravity vector and the principal normal of the wellbore, expressed in degrees;

γ_0 is the angle between the gravity vector and the binormal of the wellbore, expressed in degrees;

ϕ is the azimuth angle, expressed in degrees;

$F_{l,dp}$ is the total lateral load in the dogleg plane, expressed in newtons (pounds-force);

$F_{l,p}$ is the total lateral load perpendicular to the dogleg plane, expressed in newtons (pounds-force).

When there is no azimuth change, $\phi_1 = \phi_2 = \phi$, the above equations reduce to those of the 2-D wellbore.

5 Procedure for testing stop collars

5.1 General

For the purposes of this procedure, the term “stop collar” is used to indicate any type of device employed to prevent or limit movement of a centralizer on the casing. This includes stop collars that are independent of the centralizer and holding devices that are built into the centralizer, as in the case of solid or rigid centralizers. In this clause, the principles described for centralizers apply to other casing hardware that incorporate the use of a stop collar. Examples of these include cement baskets, scratchers, etc.

The holding device used to prevent the slippage of a centralizer can be an independent piece of equipment, as in the case of a stop collar, or can be integral within the centralizer itself. Several types are available that include the use of screws, nails and mechanical dogs. Some manufacturers also recommend the use of resins in conjunction with their particular holding device.

Regardless of the mechanism used to hold the centralizer in place, the holding device shall be capable of preventing slippage. While the holding force of the stop collar should be greater than the starting force of the centralizer, some multiplier should be applied depending on the particular well conditions.

In the case of either solid or rigid centralizers, it is recognized that these types of centralizer do not have a starting force, as they have a constant outside diameter. The minimum holding force applied to these centralizers should follow the same guidelines as a bow-type centralizer that would be used in the same hole configuration. This same recommendation also applies to other casing hardware incorporating a stop collar.

It should be noted that the data obtained for centralizer starting, running and restoring forces can vary depending on how the centralizer is installed on the casing. The use of a stop collar either as an integral part of the centralizer or with the centralizer placed over the stop collar can provide different results for some centralizers.

Further information indicates that the casing grade, mass, and surface finish can affect the results obtained from stop-collar tests. Changes in the hardness of the casing, as well as the casing wall thickness, have been shown to cause variations in the results by as much as a factor of four. It is therefore recommended that in a critical situation, the testing be performed using the same casing grade and mass as are to be used for the well.

The rate at which the load is applied during the test can have a minor effect on the results. While small changes in the loading rate should have minimal effects, shock loading can alter the results. In some instances it may be desirable to equate the loading rate to the anticipated casing running speed, and adjust the rate accordingly. There are insufficient data currently available to make a firm conclusion or recommendation on loading rates. Associated with the loading rate is the manner in which the load is applied. This test procedure incorporates a concentric loading pattern, which may not match precisely the type of


loading that can occur during actual field use. The purpose of this procedure is to provide a consistent method for performing routine tests. If the actual field conditions warrant, individual customized testing may be appropriate. Note that this is a destructive test, and may require replacement of the test casing and the stop collar following each test.

5.2 Apparatus

The test equipment used in this test shall be capable of the application of vertical loads and capable of measuring those loads and vertical displacement.

5.2.1 Test assembly, which should consist of an inner test casing and an outer sleeve (see Figure 2).

The test casing shall be within the tolerances as indicated in ISO 11960 for non-upset pipe. Burrs or similar defects should be removed prior to testing. The outer sleeve should provide a load surface on which to distribute the load to the stop device. Minor notching of the outer sleeve to allow for concentric loading is acceptable.

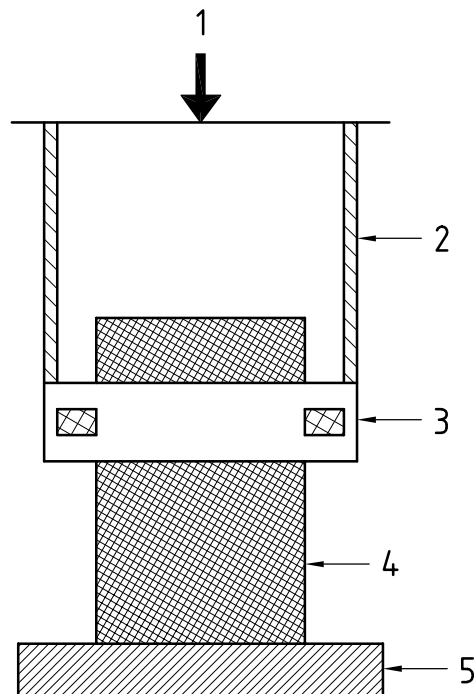

Key

- 1 applied force
- 2 outer sleeve
- 3 stop collar
- 4 test casing
- 5 rigid surface

Figure 2 — Typical test assembly

5.2.2 Instrumentation

The instrumentation should be capable of recording or otherwise indicating the application of vertical loads, including the maximum load applied during the test as well as the load at initiation of slippage (the holding force) and the slippage force range. The accuracy of load measurements should be within 5 % of the measured value.

The test stand should be instrumented to allow displacement readings of 1,6 mm (1/16 in) or less of displacement, with an accuracy of $\pm 0,8$ mm ($\pm 1/32$ in) within the range of measurement.

Measuring equipment shall be calibrated at least annually.

5.3 Test procedure

5.3.1 The stop collar should be installed on the test casing per manufacturer's recommendations. Installation position should allow for at least 102 mm (4 in) of travel during the test.

5.3.2 The outer sleeve should be placed over the test casing. This should apply a concentric load to the stop collar.

5.3.3 The outer sleeve should be continuously and slowly loaded. The applied load, plus the mass of the outer sleeve, should be recorded.

5.3.4 The test should be continued until the stop collar has been displaced at least 102 mm (4 in) or completely fails (breaks).

5.4 Reporting of test results

The following information should be reported. A typical form for test results is given in Annex A:

- a) size, mass, grade and type of surface finish of the test casing;
- b) measured inner diameter (ID) and outer diameter (OD) of the test casing, outer sleeve, and stop collar;
- c) loading rate and loading technique;
- d) holding force;
- e) slippage force range;
- f) condition of the inner test casing following the test, noting any scarring of the casing and the depth, length, and width of the scarring;
- g) orientation of the stop collar where appropriate (to be reported with stop collars that are to be installed in a particular direction);
- h) identification of any minor modifications made to the end of the outer sleeve to allow for concentric loading;
- i) stop-collar manufacturer, model number, nominal sizes, number and type of attachments, installation torque on attachment device, if applicable.

Annex A (informative)

Documentation of stop-collar test results

The form in this annex is intended for free exchange between owners/operators of the equipment or users of API RP 10D-2

Date of test: _____

A.1 Stop-collar information

Part Number: _____ Manufacturer: _____

Model Number: _____

Casing size: _____ mm (in) Installation torque (if applicable): _____

A.2 Test Specimen Number: _____

A.3 Dimensional data

A.3.1 Test assembly characteristics (see Figure 2)

Part	OD mm (in)	ID mm (in)	Mass kg (lb)
Test casing			—
Outer sleeve			
Stop collar			—

A.3.2 Test casing

A.3.2.1 Diameter: _____ mm (in)

A.3.2.2 Linear mass: _____ kg/m (lbm/ft)

A.3.2.3 Grade: _____

A.3.2.4 Surface finish: _____

A.4 Test parameters

A.4.1 Holding force (maximum load prior to slippage): _____ N (lbf)

A.4.2 Time to maximum load: _____ s

A.4.3 Load rate: _____ / _____ = _____ N/s (lbf/s)

A.4.4 Slippage force range: Max. load: _____ N (lbf); Min. load: _____ N (lbf)

A.5 Test casing inspection (post-test)

A.5.1 Scarring: _____

A.5.2 Scar depth: _____ mm (in)

A.5.3 Scar length: _____ mm (in)

A.5.4 Scar width: _____ mm (in)

A.6 Comments

Tests performed by: _____

Tests witnessed by: _____

Bibliography

- [1] API Spec 10D, *Specification for bow-spring centralizers, Fifth edition, January 1995*
- [2] ISO 10427-1:2001, *Petroleum and natural gas industries — Equipment for well cementing — Part 1: Casing bow-spring centralizers*
- [3] JUVKAM-WOLD, H.C., and BAXTER, R.L., Discussion of Optimal Spacing for Casing Centralizers, *SPE Drilling Engineering*, Dec. 1988
- [4] BLANCO, A, CICCOLA, V., and LIMONGI, E., Casing Centralization in Horizontal and Highly Inclined Wellbores, *IADC/SPE 59138*
- [5] JUVKAM-WOLD, H.C., and WU, Jiang, Casing Deflection and Centralizer Spacing Calculations, *SPE Drilling Engineering*, Dec. 1992



American Petroleum Institute

2004 Publications Order Form

Effective January 1, 2004.

API Members receive a 50% discount where applicable.

The member discount does not apply to purchases made for the purpose of resale or for incorporation into commercial products, training courses, workshops, or other commercial enterprises.

Available through Global Engineering Documents:

Phone Orders: 1-800-854-7179 (Toll-free in the U.S. and Canada)

303-397-7956 (Local and International)

Fax Orders: 303-397-2740

Online Orders: www.global.ihs.com

Date: _____

☐ **API Member** (Check if Yes)

Invoice To (☐ Check here if same as "Ship To")

Name: _____

Title: _____

Company: _____

Department: _____

Address: _____

City: _____

State/Province: _____

Zip/Postal Code: _____

Country: _____

Telephone: _____

Fax: _____

E-Mail: _____

Ship To (UPS will not deliver to a P.O. Box)

Name: _____

Title: _____

Company: _____

Department: _____

Address: _____

City: _____

State/Province: _____

Zip/Postal Code: _____

Country: _____

Telephone: _____

Fax: _____

E-Mail: _____

Quantity	Product Number	Title	SO★	Unit Price	Total

☐ **Payment Enclosed** ☐ **P.O. No.** (Enclose Copy) _____

☐ **Charge My Global Account No.** _____

☐ **VISA** ☐ **MasterCard** ☐ **American Express** ☐ **Diners Club** ☐ **Discover**

Credit Card No.: _____

Print Name (As It Appears on Card): _____

Expiration Date: _____

Signature: _____

Subtotal

Applicable Sales Tax (see below)

Rush Shipping Fee (see below)

Shipping and Handling (see below)

Total (in U.S. Dollars)

★ To be placed on **Standing Order** for future editions of this publication, place a check mark in the SO column and sign here:

Pricing and availability subject to change without notice.

Mail Orders – Payment by check or money order in U.S. dollars is required except for established accounts. State and local taxes, \$10 processing fee*, and 5% shipping must be added. Send mail orders to: **API Publications, Global Engineering Documents, 15 Inverness Way East, M/S C303B, Englewood, CO 80112-5776, USA.**

Purchase Orders – Purchase orders are accepted from established accounts. Invoice will include actual freight cost, a \$10 processing fee*, plus state and local taxes.

Telephone Orders – If ordering by telephone, a \$10 processing fee* and actual freight costs will be added to the order.

Sales Tax – All U.S. purchases must include applicable state and local sales tax. Customers claiming tax-exempt status must provide Global with a copy of their exemption certificate.

Shipping (U.S. Orders) – Orders shipped within the U.S. are sent via traceable means. Most orders are shipped the same day. Subscription updates are sent by First-Class Mail. Other options, including next-day service, air service, and fax transmission are available at additional cost. Call 1-800-854-7179 for more information.

Shipping (International Orders) – Standard international shipping is by air express courier service. Subscription updates are sent by World Mail. Normal delivery is 3-4 days from shipping date.

Rush Shipping Fee – Next Day Delivery orders charge is \$20 in addition to the carrier charges. Next Day Delivery orders must be placed by 2:00 p.m. MST to ensure overnight delivery.

Returns – All returns must be pre-approved by calling Global's Customer Service Department at 1-800-624-3974 for information and assistance. There may be a 15% restocking fee. Special order items, electronic documents, and age-dated materials are non-returnable.


***Minimum Order** – There is a \$50 minimum for all orders containing hardcopy documents. The \$50 minimum applies to the order subtotal including the \$10 processing fee, excluding any applicable taxes and freight charges. If the total cost of the documents on the order plus the \$10 processing fee is less than \$50, the processing fee will be increased to bring the order amount up to the \$50 minimum. This processing fee will be applied before any applicable deposit account, quantity or member discounts have been applied. There is no minimum for orders containing only electronically delivered documents.

There's more where this came from.

The American Petroleum Institute provides additional resources and programs to the oil and natural gas industry which are based on API® Standards. For more information, contact:

- | | |
|---|--|
| • API Monogram® Licensing Program | Phone: 202-962-4791
Fax: 202-682-8070 |
| • American Petroleum Institute Quality Registrar (APIQR®) | Phone: 202-962-4791
Fax: 202-682-8070 |
| • API Spec Q1® Registration | Phone: 202-962-4791
Fax: 202-682-8070 |
| • API Perforator Design Registration | Phone: 202-962-4791
Fax: 202-682-8070 |
| • API Training Provider Certification Program | Phone: 202-682-8490
Fax: 202-682-8070 |
| • Individual Certification Programs | Phone: 202-682-8064
Fax: 202-682-8348 |
| • Engine Oil Licensing and Certification System (EOLCS) | Phone: 202-682-8516
Fax: 202-962-4739 |
| • API PetroTEAM™
(Training, Education and Meetings) | Phone: 202-682-8195
Fax: 202-682-8222 |

Check out the API Publications, Programs, and Services Catalog online at www.api.org.

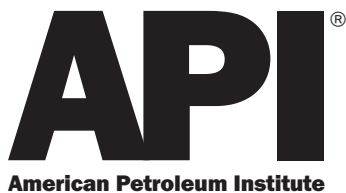

Helping You Get The Job Done Right.®

Additional copies are available through Global Engineering Documents at (800) 854-7179 or (303) 397-7956

Information about API Publications, Programs and Services is available on the World Wide Web at <http://www.api.org>



1220 L Street, Northwest
Washington, D.C. 20005-4070
202-682-8000

Product No: GG10D21