

ASME MFC-21.2–2010

Measurement of Fluid Flow by Means of Thermal Dispersion Mass Flowmeters

AN AMERICAN NATIONAL STANDARD



Copyright © 2011 by the American Society of Mechanical Engineers.
No reproduction may be made of this material without written consent of ASME.



INTENTIONALLY LEFT BLANK



ASME MFC-21.2–2010

Measurement of Fluid Flow by Means of Thermal Dispersion Mass Flowmeters

AN AMERICAN NATIONAL STANDARD



Three Park Avenue • New York, NY • 10016 USA

Copyright © 2011 by the American Society of Mechanical Engineers.
No reproduction may be made of this material without written consent of ASME.



Date of Issuance: January 10, 2011

This Standard will be revised when the Society approves the issuance of a new edition. There will be no addenda issued to this edition.

ASME issues written replies to inquiries concerning interpretations of technical aspects of this document. Periodically certain actions of the ASME MFC Committee may be published as Cases. Cases and interpretations are published on the ASME Web site under the Committee Pages at <http://cstools.asme.org> as they are issued.

ASME is the registered trademark of The American Society of Mechanical Engineers.

This code or standard was developed under procedures accredited as meeting the criteria for American National Standards. The Standards Committee that approved the code or standard was balanced to assure that individuals from competent and concerned interests have had an opportunity to participate. The proposed code or standard was made available for public review and comment that provides an opportunity for additional public input from industry, academia, regulatory agencies, and the public-at-large.

ASME does not “approve,” “rate,” or “endorse” any item, construction, proprietary device, or activity.

ASME does not take any position with respect to the validity of any patent rights asserted in connection with any items mentioned in this document, and does not undertake to insure anyone utilizing a standard against liability for infringement of any applicable letters patent, nor assume any such liability. Users of a code or standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, is entirely their own responsibility.

Participation by federal agency representative(s) or person(s) affiliated with industry is not to be interpreted as government or industry endorsement of this code or standard.

ASME accepts responsibility for only those interpretations of this document issued in accordance with the established ASME procedures and policies, which precludes the issuance of interpretations by individuals.

No part of this document may be reproduced in any form,
in an electronic retrieval system or otherwise,
without the prior written permission of the publisher.

The American Society of Mechanical Engineers
Three Park Avenue, New York, NY 10016-5990

Copyright © 2011 by
THE AMERICAN SOCIETY OF MECHANICAL ENGINEERS
All rights reserved
Printed in U.S.A.



CONTENTS

Foreword	iv
Committee Roster	v
Correspondence With the MFC Committee	vi
1 Scope	1
2 Terminology and Symbols	1
3 General Description	5
4 Principle of Operation	8
5 Guidelines for Flowmeter Selection	12
6 Guidelines for Installation and Applications	14
7 Inspection and Compliance	18
8 Safety	18
9 References	19
Figures	
3.1-1 The Major Components of Two Configurations of Thermal Dispersion Mass Flowmeters	6
3.2-1 Flow Sensor of Thermal Dispersion Mass Flowmeters	7
3.3-1 Two Modes of Flow Sensor Operation	9
4-1 Principle of Operation	9
Tables	
2.3-1 Symbols	2
2.4-1 Abbreviations	4
6.1.4-1 Straight Pipe Length Requirements for an In-Line Flowmeter With a Built-In Flow Conditioner	16
6.1.4-2 Straight Pipe Length Requirements for Insertion Flowmeters With No Flow Conditioning	16
Mandatory Appendix	
I Flow Calibration	21
Nonmandatory Appendices	
A In-Line Flowmeter Sizing and Permanent Pressure Loss	25
B Accuracy and Uncertainty	27



FOREWORD

Thermal dispersion mass flowmeters comprise a family of instruments for the measurement of the total mass flow rate of a fluid, primarily gases, flowing through closed conduits.

The operation of thermal dispersion mass flowmeters is attributed to L.V. King who, in 1914 [1], published his famous King's Law revealing how a heated wire immersed in a fluid flow measures the mass velocity at a point in the flow. King called his instrument a "hot-wire anemometer." However, it was not until the 1960s and 1970s that industrial-grade thermal dispersion mass flowmeters finally emerged.

This Standard covers the thermal dispersion type of thermal mass flowmeter. A companion standard, ASME MFC 21.1, Measurement of Fluid Flow by Means of Capillary Tube Thermal Mass Flowmeters and Controllers, covers the other most commonly used type of thermal mass flowmeter. Both types measure fluid mass flow rate by means of the heat convected from a heated surface to the flowing fluid. In the case of the thermal dispersion, or immersible, type of flowmeter, the heat is transferred to the boundary layer of the fluid flowing over the heated surface. In the case of the capillary tube type of flowmeter the heat is transferred to the bulk of the fluid flowing through a small heated capillary tube. The principles of operation of the two types are both thermal in nature, but are so substantially different that two separate standards are required. Additionally, their applications are much different. Thermal dispersion flowmeters are commonly used for general industrial gas-flow applications in pipes and ducts, whereas capillary tube flowmeters are primarily used for smaller flows of clean gases in tubes.

Suggestions for improvement of this Standard will be welcomed. They should be sent to The American Society of Mechanical Engineers; Attn: Secretary, MFC Standards Committee; Three Park Avenue; New York, NY 10016-5990.

This Standard was approved as an American National Standard on June 24, 2010.



ASME MFC COMMITTEE

Measurement of Fluid Flow in Closed Conduits

(The following is the roster of the Committee at the time of approval of this Standard.)

STANDARDS COMMITTEE OFFICERS

R. J. DeBoom, *Chair*
Z. D. Husain, *Vice Chair*
D. C. Wyatt, *Vice Chair*
C. J. Gomez, *Secretary*

STANDARDS COMMITTEE PERSONNEL

C. J. Blechinger, *Honorary Member*, Consultant
R. M. Bough, Rolls-Royce Motor Cars
M. S. Carter, Flow Systems, Inc.
G. P. Corpron, *Honorary Member*, Consultant
R. J. DeBoom, Consultant
D. Faber, *Contributing Member*, Badger Meter, Inc.
C. J. Gomez, The American Society of Mechanical Engineers
F. D. Goodson, Emerson Process
Z. D. Husain, Chevron Corp.
C. G. Langford, *Honorary Member*, Consultant
T. O. Maginnis, Consultant
W. M. Mattar, Invensys/Foxboro Co.

G. E. Mattingly, The Catholic University of America
D. R. Mesnard, Consultant
R. W. Miller, *Honorary Member*, R. W. Miller & Associates, Inc.
A. Quraishi, American Gas Association
W. Seidl, Colorado Engineering Experiment Station, Inc.
D. W. Spitzer, *Contributing Member*, Spitzer and Boyes LLC
R. N. Steven, Colorado Engineering Experiment Station, Inc.
T. M. Kegel, *Alternate*, Colorado Engineering Experiment Station, Inc.
J. H. Vignos, *Honorary Member*, Consultant
D. E. Wiklund, Rosemount, Inc.
J. D. Wright, *Contributing Member*, NIST
D. C. Wyatt, Wyatt Engineering

SUBCOMMITTEE 21 — THERMAL MASS FLOWMETERS

R. J. DeBoom, *Chair*, Consultant
T. O. Maginnis, *Vice Chair*, Consultant
Z. D. Husain, Chevron Corp.

J. G. Olin, Sierra Instruments, Inc.
B. K. Rao, Consultant



CORRESPONDENCE WITH THE MFC COMMITTEE

General. ASME Standards are developed and maintained with the intent to represent the consensus of concerned interests. As such, users of this Standard may interact with the Committee by requesting interpretations, proposing revisions, and attending Committee meetings. Correspondence should be addressed to:

Secretary, MFC Standards Committee
The American Society of Mechanical Engineers
Three Park Avenue
New York, NY 10016-5990
<http://go.asme.org/Inquiry>

Proposing Revisions. Revisions are made periodically to the Standard to incorporate changes that appear necessary or desirable, as demonstrated by the experience gained from the application of the Standard. Approved revisions will be published periodically.

The Committee welcomes proposals for revisions to this Standard. Such proposals should be as specific as possible, citing the paragraph number(s), the proposed wording, and a detailed description of the reasons for the proposal, including any pertinent documentation.

Proposing a Case. Cases may be issued for the purpose of providing alternative rules when justified, to permit early implementation of an approved revision when the need is urgent, or to provide rules not covered by existing provisions. Cases are effective immediately upon ASME approval and shall be posted on the ASME Committee Web page.

Requests for Cases shall provide a Statement of Need and Background Information. The request should identify the Standard, the paragraph, figure or table number(s), and be written as a Question and Reply in the same format as existing Cases. Requests for Cases should also indicate the applicable edition(s) of the Standard to which the proposed Case applies.

Interpretations. Upon request, the MFC Committee will render an interpretation of any requirement of the Standard. Interpretations can only be rendered in response to a written request sent to the Secretary of the MFC Standards Committee.

The request for interpretation should be clear and unambiguous. It is further recommended that the inquirer submit his/her request in the following format:

Subject:	Cite the applicable paragraph number(s) and the topic of the inquiry.
Edition:	Cite the applicable edition of the Standard for which the interpretation is being requested.
Question:	Phrase the question as a request for an interpretation of a specific requirement suitable for general understanding and use, not as a request for an approval of a proprietary design or situation. The inquirer may also include any plans or drawings, that are necessary to explain the question; however, they should not contain proprietary names or information.

Requests that are not in this format may be rewritten in the appropriate format by the Committee prior to being answered, which may inadvertently change the intent of the original request.

ASME procedures provide for reconsideration of any interpretation when or if additional information that might affect an interpretation is available. Further, persons aggrieved by an interpretation may appeal to the cognizant ASME Committee or Subcommittee. ASME does not “approve,” “certify,” “rate,” or “endorse” any item, construction, proprietary device, or activity.

Attending Committee Meetings. The MFC Standards Committee regularly holds meetings that are open to the public. Persons wishing to attend any meeting should contact the Secretary of the MFC Standards Committee.



MEASUREMENT OF FLUID FLOW BY MEANS OF THERMAL DISPERSION MASS FLOWMETERS

1 SCOPE

This Standard establishes common terminology and gives guidelines for the quality, description, principle of operation, selection, installation, and flow calibration of thermal dispersion flowmeters for the measurement of the mass flow rate, and to a lesser extent, the volumetric flow rate, of the flow of a fluid in a closed conduit. Multivariable versions additionally measure fluid temperature. Thermal dispersion mass flowmeters are applicable to the flow of single-phase pure gases and gas mixtures of known composition and, less commonly, to single-phase liquids of known composition. Companion standard ASME MFC-21.1 covers capillary tube type thermal mass flowmeters and controllers.

2 TERMINOLOGY AND SYMBOLS

(a) Paragraph 2.1 lists definitions from ASME MFC-1M used in ASME MFC-21.2.

(b) Paragraph 2.2 lists definitions specific to this Standard.

(c) Paragraph 2.3 lists symbols (see Table 2.3-1) used in this Standard (see notes and superscripts).

(d) Paragraph 2.4 lists abbreviations (see Table 2.4-1) used in this Standard.

2.1 Definitions Copied From ASME MFC-1M

accuracy: the degree of freedom from error; the degree of conformity of the indicated value to the true value of the measured quantity.

calibration: the experimental determination of the relationship between the quantity being measured and the device that measures it, usually by comparison with a standard. Also, the act of adjusting the output of a device to bring it to a desired value, within a specified tolerance, for a particular value of the input.

cavitation: the implosion of vapor bubbles formed after flashing when the local pressure rises above the vapor pressure of a liquid. (See also *flashing*.)

flashing: the formation of vapor bubbles in a liquid when the local pressure falls to or below the vapor pressure of the liquid, often due to local lowering of pressure because of an increase in the liquid velocity. (See also *cavitation*.)

flow profile: graphic representation of the velocity distribution.

fully developed velocity distribution: a velocity distribution, in a straight length of pipe, that has zero radial and azimuthal fluid velocity components and an axisymmetric axial velocity profile that is independent of axial position along the pipe.

rangeability (turndown): flowmeter rangeability is the ratio of the maximum to minimum flow rates or Reynolds number in the range over which the meter meets a specified uncertainty (accuracy).

repeatability (qualitative): the closeness of agreement among a series of results obtained with the same method on identical test material, under the same conditions (same operator, same apparatus, same laboratory, and short intervals of time). [See also *repeatability (quantitative)*.]

repeatability (quantitative): the value below which the absolute difference between any two single test results obtained under same conditions may be expected to lie with a specified probability. In the absence of other indications, the probability is 95%. [See also *repeatability (qualitative)*.]

reproducibility (quantitative): the closeness of agreement between results obtained when the conditions of measurement differ; for example, with respect to different test apparatus, operators, facilities, time intervals, etc.

swirling flow: flow that has axial and circumferential velocity components.

transmitter (secondary device): electronic system providing the drive and transforming the signals from the flow sensor to give output(s) of measured and inferred parameters; it also provides corrections derived from parameters such as temperature.

uncertainty interval, u : an estimate of the error band, centered about the measurement, within which the true value must fall with a specified probability.

2.2 Definitions Specific to This Document

base conditions: the conditions of temperature and pressure to which measured volumes are to be corrected (same as *Reference* or *Standard Conditions*).



Table 2.3-1 Symbols

Symbol	Description (First Use)	Dimensions [Note (1)]	SI Units [Note (2)]	USC Units [Note (2)]
$Abs()$	Absolute value of the quantity in parentheses [eq. (B-1)]	dim-less		
A_e	External surface area of the heated section of the velocity sensor [eq. (4-2)]	L^2	m^2	$ft^2, in.^2$
A_{fs}	Accuracy of flowmeter, percent of full scale [eq. (5-2)]	dim-less	% fs	% fs
A_{pipe}	Cross-sectional area of the flow conduit or flow body [eq. (4-6)]	L^2	m^2	$ft^2, in.^2$
A_r	Accuracy of flowmeter, percent of reading [eq. (5-1)]	dim-less	% r	% r
A_t	Overall accuracy of flowmeter, in percent of reading [eq. (5-1)]	dim-less	% r	% r
atm	Atmospheric pressure at base conditions, 101,325 Pa	$ML^{-1}T^{-2}$	Pa, bar	psi
b_i	Gas factors, $i = 1, 2, \dots, 5$ [eq. (4-10)]	dim-less		
C_p	Pressure influence coefficient (para. 5.6.1)	$M^{-1}LT^2$	% r/bar	% r/psi
c_p	Coefficient of specific heat of the fluid at constant pressure [eq. (4-9)]	$L^2T^{-2}K^{-1}$	J/kg·K	Btu/lb·°F
C_T	Temperature influence coefficient (para. 5.6.1)	K^{-1}	% r/K	% r/°F
D	Outside diameter of the velocity sensor [eq. (4-2)]	L	m	ft, in.
F_c	Conduit factor [eq. (4-8)]	dim-less		
$f()$	Function of terms in parentheses [eq. (4-9)]	dim-less		
h	Film coefficient for convective heat transfer from the heated section of the velocity sensor [eq. (4-3)]	$MT^{-3}K^{-1}$	$W/m^2 \cdot K$	Btu/h·ft ² ·°F
h_e	Equivalent film coefficient for convective heat transfer from the heated section of the velocity sensor [eq. (4-2)]	$MT^{-3}K^{-1}$	$W/m^2 \cdot K$	Btu/h·ft ² ·°F
I	Electrical current input to T_1 RTD in the heated section of the velocity sensor (para. 3.5.2)	amperes	A	A
k_f	Thermal conductivity of the fluid [eq. (4-9)]	$MLT^{-3}K^{-1}$	$W/m \cdot K$	Btu/h·ft·°F
L	Length of the heated section of the velocity sensor [eq. (4-2)]	L	m	ft, in.
M	Molecular weight of the gas [eq. (4-21)]	---	kg/kgmole	lb/lbmole
N	Number of equal areas in the cross-sectional area A_{pipe} of a flow conduit [eq. (4-20)]	dim-less		
Nu	Nusselt number [eq. (4-9)]	dim-less		
n	Number of input variables [eq. (B-2)]	dim-less		
P	Static pressure of the flowing fluid [eq. (4-21)]	$ML^{-1}T^{-2}$	Pa, bar	psi
P_b	Base static pressure of the flowing fluid (para. 4.7.3) – “normal” base conditions: $P_b = P_n = 101,325$ Pa (1 atm) – “standard” base conditions: $P_b = P_s = 101,325$ Pa (1 atm)	$ML^{-1}T^{-2}$	Pa, bar	psi
P_L	The upper or lower limit of the pressure flow calibration reference condition range [eq. (B-1)]	$ML^{-1}T^{-2}$	Pa, bar	psi
Pr	Prandtl number [eq. (4-9)]	dim-less		
Q	Heat convected away from the heated section of the velocity sensor by the fluid [eq. (4-1)]	ML^2T^{-3}	W	Btu/h
Q_L	Stem conduction heat loss [eq. (4-1)]	ML^2T^{-3}	W	Btu/h
q_m	Mass flow rate of the fluid (para. 3.2)	MT^{-1}	kg/s	lb/s, lb/min
$q_{m,fs}$	Full scale mass flow rate of the flowmeter [eq. (5-2)]	MT^{-1}	kg/s	lb/s, lb/min
$q_{m,i}$	Mass flow rate of the fluid measured by flow sensor i [eq. (4-20)]	MT^{-1}	kg/s	lb/s, lb/min
q_v	Volumetric flow rate of the fluid [eq. (4-16)]	L^3T^{-1}	m^3/s	ft^3/min
$q_{v,b}$	Volumetric flow rate of the fluid referenced to base (“b”) conditions [eq. (4-17)]	L^3T^{-1}	bm^3/s	bft^3/min
R	Universal gas constant [eq. (4-21)]	---	$m^3 \cdot bar / (kg \cdot mole \cdot K)$	$ft \cdot lbf / (lbmole \cdot ^\circ R)$
Re	Reynolds number of the velocity sensor [eq. (4-9)]	dim-less		
Re_{pipe}	Reynolds number of the flow conduit, pipe, or flow body [eq. (4-8)]	dim-less		
R_s	Skin thermal resistance [eq. (4-5)]	$M^{-1}L^{-2}T^3K$	K/W	°F/(Btu/h)
R_1	Electrical resistance of the T_1 RTD [eq. (4-1)]	ohms	ohms	ohms
S_i	Sensitivity coefficient of q_m to input variable x_i [eq. (B-3)]	varies		
T	Temperature of a gas in the absolute scale [eq. (4-21)]	K	K	°R



Table 2.3-1 Symbols (Cont'd)

Symbol	Description (First Use)	Dimensions [Note (1)]	SI Units [Note (2)]	USC Units [Note (2)]
T_b	Base temperature of the flowing fluid (para. 4.7.3) – “normal” base conditions: $T_b = T_n = 0^\circ\text{C}$ – “standard” base conditions: $T_b = T_s = 21.1^\circ\text{C}$ (or 70°F)	K	K, $^\circ\text{C}$	$^\circ\text{F}$
T_e	Average external surface temperature over the length of the heated section of the velocity sensor [eq. (4-5)]	K	K, $^\circ\text{C}$	$^\circ\text{F}$
T_f	Temperature of the flowing fluid measured by the T_f RTD in the fluid temperature sensor (para. 3.2)	K	K, $^\circ\text{C}$	$^\circ\text{F}$
T_L	The upper or lower limit of the temperature flow calibration reference condition range [eq. (B-1)]	K	K, $^\circ\text{C}$	$^\circ\text{F}$
T_1	Average temperature of the T_1 RTD over the length L of the heated section of the velocity sensor (para. 3.2)	K	K, $^\circ\text{C}$	$^\circ\text{F}$
t	The factor in uncertainty from the students t distribution [eq. (B-3)]	dim-less		
t_{68}	The factor in uncertainty yielding a 68% confidence level [eq. (B-3)]	dim-less		
t_{95}	The factor in uncertainty yielding a 95% confidence level [eq. (B-3)]	dim-less		
$u(q_m)$	Uncertainty in mass flow rate q_m [eq. (B-3)]	MT^{-1}	kg/s	lb/s, lb/min
$u(x_i)$	Uncertainty in input variable x_i [eq. (B-3)]	varies		
V	Point velocity of the fluid [eq. (4-7)]	LT^{-1}	m/s	ft/min
V_{ave}	Average velocity of the fluid over area A_{pipe} [eq. (4-6)]	LT^{-1}	m/s	ft/min
$V_{\text{ave}, b}$	Average velocity of the fluid over area A_{pipe} referenced to base (“b”) conditions [eq. (4-6)]	LT^{-1}	bm/s	bft/min
V_b	Point velocity of the fluid referenced to base (“b”) conditions [eq. (4-7)]	LT^{-1}	bm/s	bft/min
Vol	Displaced volume (para. I-3.3.2)	L^3	m^3	ft^3
W	Electrical input to the T_1 RTD in the heated section of the velocity sensor (para. 3.5.1)	ML^2T^{-3}	W	Btu/h
x_i	Input variable, $i = 1, 2, \dots, n$ [eq. (B-2)]	varies		
Z	Compressibility of a gas [eq. (4-21)]	dim-less		

Greek Symbols				
δ	Partial differential [eq. (B-3)]	dim-less		
ΔT	Differential temperature $T_1 - T_f$ (para. 3.5.1)	K	K, $^\circ\text{C}$	$^\circ\text{F}$
Δt	Transit time (para. I-3.3.2)	T	s	s
μ	Absolute viscosity of the fluid [eq. (4.9)]	$\text{ML}^{-1}\text{T}^{-1}$	kg/s·m	lb/ft·h
ρ	Mass density of the fluid [eq. (4.6)]	ML^{-3}	kg/m^3	lb/ft^3
ρ_b	Mass density of the fluid that is referenced to base (“b”) conditions and is a constant [eq. (4.6)]	ML^{-3}	kg/m^3	lb/ft^3
ρV	Mass velocity (para. 4.6.1)	$\text{ML}^{-2}\text{T}^{-1}$	$\text{kg}/\text{s}\cdot\text{m}^2$	$\text{lb}/\text{min}\cdot\text{ft}^2$
$\Sigma ()$	Sum of terms in parentheses [eq. (B-3)]	dim-less		

Subscripts		
ave	Average value over the cross-sectional area of a pipe or flow conduit	dim-less
b	Referenced to base conditions of T_b and P_b	dim-less
f	Fluid or flow	dim-less
fs	Full scale value	dim-less
m	Mass flow rate	dim-less
n	Normal base conditions of $T_b = 0^\circ\text{C}$ and $P_b = 1$ atm	dim-less
pipe	Pipe or flow conduit	dim-less
s	Standard base conditions of $T_b = 21.1^\circ\text{C}$ (or 70°F) and $P_b = 1$ atm	dim-less
v	Volumetric flow rate	dim-less
1	Refers to the T_1 RTD	dim-less

NOTES:

- (1) M = mass; l = Length; T = time; K = thermodynamic temperature (degrees Kelvin); dim-less = dimensionless; varies = dimensions depend on the quantity to which the symbol refers.
- (2) fs = full scale; r = reading; Pa = Pascal; b = referenced to base conditions; lb = lbm = pound mass; $^\circ\text{R}$ = degrees Rankin; W = watts.



Table 2.4-1 Abbreviations

Abbreviation	Description
b	refers to base conditions
bara	bars, absolute
barg	bars, gage
bm/s	meters per second referenced to base “b” conditions
bm ³ /s	cubic meters per second referenced to base “b” conditions
DN	European piping size (diameter nominal, millimeters)
normal m/s	meters per second referenced to “normal” base conditions
normal m ³ /s	cubic meters per second referenced to “normal” base conditions
PN	European pressure standard (pressure nominal, bars)
PRTD	platinum resistance temperature detector
psi	pounds force per square inch
psia	pounds force per square inch, absolute
psig	pounds force per square inch, gage
RTD	resistance temperature detector
Scfm	standard cubic feet per minute referenced to “standard” base conditions
Sfpm	standard feet per minute referenced to “standard” base conditions
T _f RTD	RTD in fluid temperature sensor
T ₁ RTD	RTD in heated section of velocity sensor

base pressure: the pressure base condition of a fluid. Typically, the “normal” and “standard” base conditions are both 101.325 kPa, 1 atm (14.69595 psia). (See also *base conditions*.)

base temperature: the temperature base condition of a fluid. Typically, the “normal” base temperature is 0°C, and the “standard” base temperature is 21.1°C (70°F). (See also *base conditions*.)

batching flow calibration standard: a flow calibration standard that provides an output signal only when a discrete quantity, or batch, of fluid fills the flow calibration standard. (See also *flow calibration standard*.)

conduit factor: a correction factor for the velocity distribution in a flow conduit that is the ratio of the average velocity over the cross-sectional area of the conduit to its centerline velocity. (See also *fully developed velocity distribution*.)

flow calibration facility: an open or closed loop piping system used for the determination of the relationship between flow rate and the output of the flowmeter under test. At a minimum, the flow calibration facility has the following components: flow generator, flow calibration standard, and the flowmeter under test. (See also *calibration*.)

flow calibration standard: an in-line or batching flowmeter used in a flow calibration facility as a secondary, or transfer, standard for the flow calibration of the flowmeter under test. The flow calibration standard must be traceable to a recognized national or international measurement standard. (See also *calibration*; *in-line flow calibration standard*; and *batching flow calibration standard*.)

flow conditioner: a device installed in a pipeline upstream and downstream of a flowmeter (or built into an in-line flowmeter) for the purpose of normalizing or regulating the flow profile and reducing swirling flow.

flow sensor: a fluid mass flow rate sensing subassembly in a thermal dispersion mass flowmeter consisting of a fluid temperature sensor and an electronically heated velocity sensor, both immersed in, and/or exposed to, the flowing fluid.

in-line flow calibration standard: a flow calibration standard that provides a continuous output signal. (See also *flow calibration standard*.)

in-line flowmeter: a flowmeter that is installed directly in a pipeline that is running full and generates an output with a known relationship to the fluid flow in the pipe.

insertion flowmeter: a flowmeter that is inserted into the pipeline and measures flow velocity at a point or over a limited area or volume of the entire cross-sectional area of the pipe.

installation effect: any difference in performance of the flowmeter arising between the flow calibration under ideal conditions and the actual conditions of use. This difference may be caused by different flow conditions due to changes in flow profile, perturbations, or by different working regimes (pulsations, intermittent flow, alternating flow, vibrations, etc.).

linearity: the consistency of the change in the scaled output of the flowmeter for a related scaled change in the input of the flowmeter.

normal volume flow: in this document normal volume flow rate is interchangeably used as mass flow rate because the normal base conditions density of the flowing fluid is defined in the industry that is expected to be the predominant user of this Standard.

Nusselt number: a dimensionless number that is the ratio of convective to conductive heat transfer across (normal to) the boundary.



permanent pressure loss: the difference between the upstream pressure and the downstream pressure of the flowmeter after recovery.

Prandtl number: a dimensionless number approximating the ratio of momentum diffusivity (kinematic viscosity) to thermal diffusivity.

resistance temperature detector: a sensor that measures temperature by means of the increase in its electrical resistance as temperature increases.

sensitivity: the slope of the raw nonlinear flow calibration curve of the output signal versus mass flow rate.

Reynolds number: a dimensionless number that is the ratio of inertia forces to viscous forces.

skin resistance: the thermal resistance of the intervening layers of material, or skin, in the heated section of the velocity sensor that exists between the embedded heated resistance temperature detector and the external surface. (See also *resistance temperature detector*.)

stem conduction: the heat lost from the heated section of the velocity sensor that is conducted through the stem of the velocity sensor to the environment external to the flowmeter.

temperature compensation: means in the transmitter for correcting the output signal for changes in fluid temperature. (See also *transmitter*.)

volumetric prover: the use of a calibrated volume tank, gas density, and most generally a diverter valve, to calibrate a flowmeter. Bell provers and piston provers are typical volumetric provers. (See also *batching flow calibration standards*.)

2.3 Symbols Used in This Standard

See Table 2.3-1 for symbols used in this Standard.

2.4 Abbreviations Used in This Standard

See Table 2.4-1 for the abbreviations used in this Standard.

3 GENERAL DESCRIPTION

Thermal dispersion mass flowmeters measure the mass flow rate of a fluid or a mixture of fluids of known composition flowing through a closed conduit. Multi-variable versions also measure the volumetric flow rate and fluid temperature. This section describes the configurations and major components of thermal dispersion mass flowmeters.

3.1 Configurations

Thermal dispersion mass flowmeters have two primary configurations: in-line and insertion. Figure 3.1-1 shows the two configurations and their major components.

3.1.1 In-Line Flowmeter Configuration. In-line thermal dispersion mass flowmeters typically are applied to pipes and conduits with diameters (or equivalent diameters for noncircular cross sections) less than about 200 mm (8 in.). As shown in Fig. 3.1-1, in-line flowmeters consist of the following major components: flow body, process connections, flow sensor, flow sensor probe, flow conditioner, transmitter enclosure, and transmitter. In-line flowmeters measure the mass flow rate flowing through the pipe.

The process connections are flanged, pipe threads, or compression fittings. A separate or built-in flow conditioner upstream of the flow sensor reduces the straight length requirement of pipe upstream of the flow body required to achieve a flow-profile independent of upstream flow disturbances and nonuniformities.

3.1.2 Insertion Flowmeter Configuration. Insertion flowmeters [4] typically are applied to pipes and flow conduits with diameters (or equivalent diameters for noncircular cross sections) greater than about 200 mm (8 in.). Because they are more economical than in-line flowmeters, they also have found applications in smaller pipes or conduits and wide use as flow switches.

Insertion flowmeters have the same major components as in-line flowmeters, but do not have a flow body. Their process connection is a compression fitting or flange that is welded onto, or threaded into, an existing process fluid conduit. Insertion flowmeters measure the mass velocity at a point in the conduit's cross-sectional area, but usually are flow calibrated to measure the mass flow rate flowing through the conduit.



Multipoint insertion flowmeters measure the mass velocity at several points in the cross-sectional area of large pipes, ducts, and stacks. The mass flow rate through the entire conduit is the average mass velocity multiplied by the cross-sectional area [5].

3.2 Flow Sensor

As shown in Figs. 3.1-1 and 3.2-1, the flow sensor of both in-line and insertion configurations have an electrically heated velocity sensor and a fluid temperature sensor immersed in the flowing fluid. For that reason thermal dispersion mass flowmeters are also called "immersible" thermal mass flowmeters. Reference [6] describes the several types of flow sensors used by immersible thermal mass flowmeters.

The heated section of the velocity sensor consists of a self-heated temperature sensor that both heats the sensor and measures its own average temperature, T_1 . The fluid temperature sensor is not self-heated and measures the temperature, T_f , of the flowing fluid. For higher accuracy applications, the sensor elements in the velocity sensor and the fluid temperature sensor should be wire-wound or thin-film platinum resistive temperature detectors (RTDs). The electrical resistance of RTDs increases as temperature increases. The platinum RTD

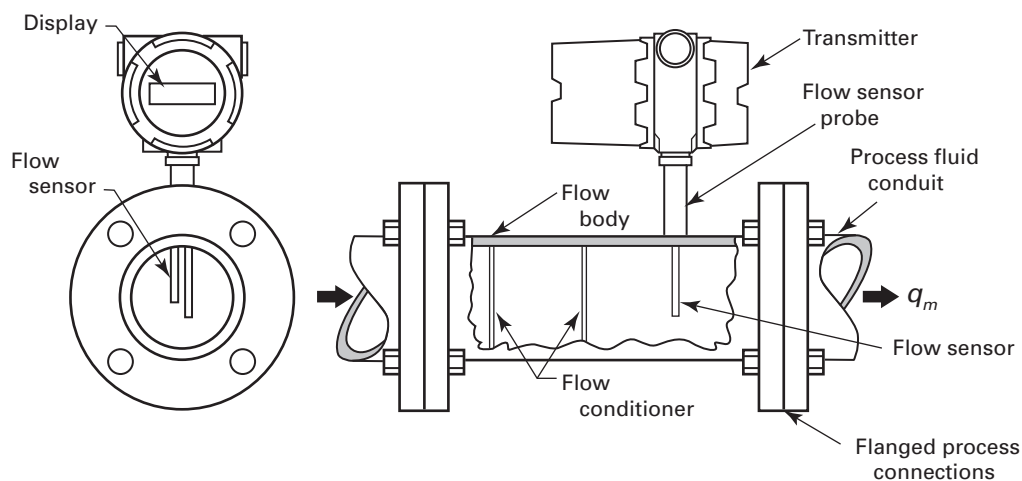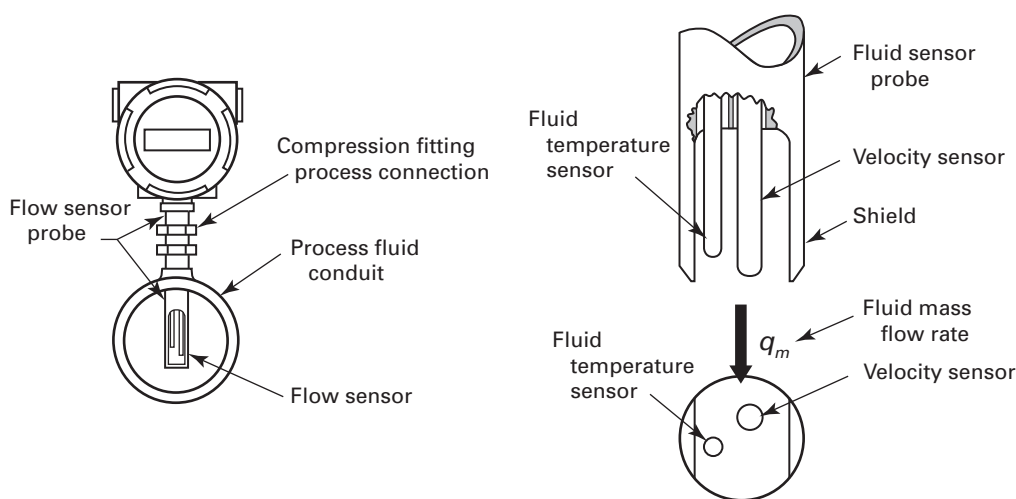

Fig. 3.1-1 The Major Components of Two Configurations of Thermal Dispersion Mass Flowmeters**(a) In-Line Configuration With Meter-Mounted Transmitter****(b) Insertion Configuration, Installed****(c) Detail of Flow Sensor for Both Configurations**

sensor element in the velocity sensor is called the " T_1 RTD." The platinum RTD sensor element in the fluid temperature sensor is called the " T_f RTD." Other types of sensor elements such as thermistors, thermocouples, and microelectronic machined devices are used by some manufacturers.


In traditional velocity sensors, the T_1 RTD sensor is potted into the tip of the tubular sheath. The potting compound, or filler material, typically is ceramic cement or epoxy. Another category of flow sensors avoids the use of potting compounds by tightly fitting a wire wound platinum RTD into the tip of the sheath.

The flow sensors of most industrial-grade thermal dispersion mass flowmeters have cylindrical single-ended velocity and fluid temperature sensors mounted

side-by-side as shown in Figs. 3.1-1 and 3.2-1. Both sensors are sheathed in corrosion-resistant tubular metallic sheaths. The principle of operation described in section 4 is based on this most common type of flow sensor construction.

Light-duty flowmeters have unsheathed single-ended, side-by-side sensors immersed in the flow or a piggy-back construction that has coaxial velocity and fluid temperature sensors with the velocity sensor mounted on the end.

In yet another flow sensor construction for in-line meters, the flow sensor is embedded in the wall of the flow body and is not immersed in the flowing fluid [7]. Here the flow sensor consists of a heater element with adjacent upstream and downstream temperature sensor

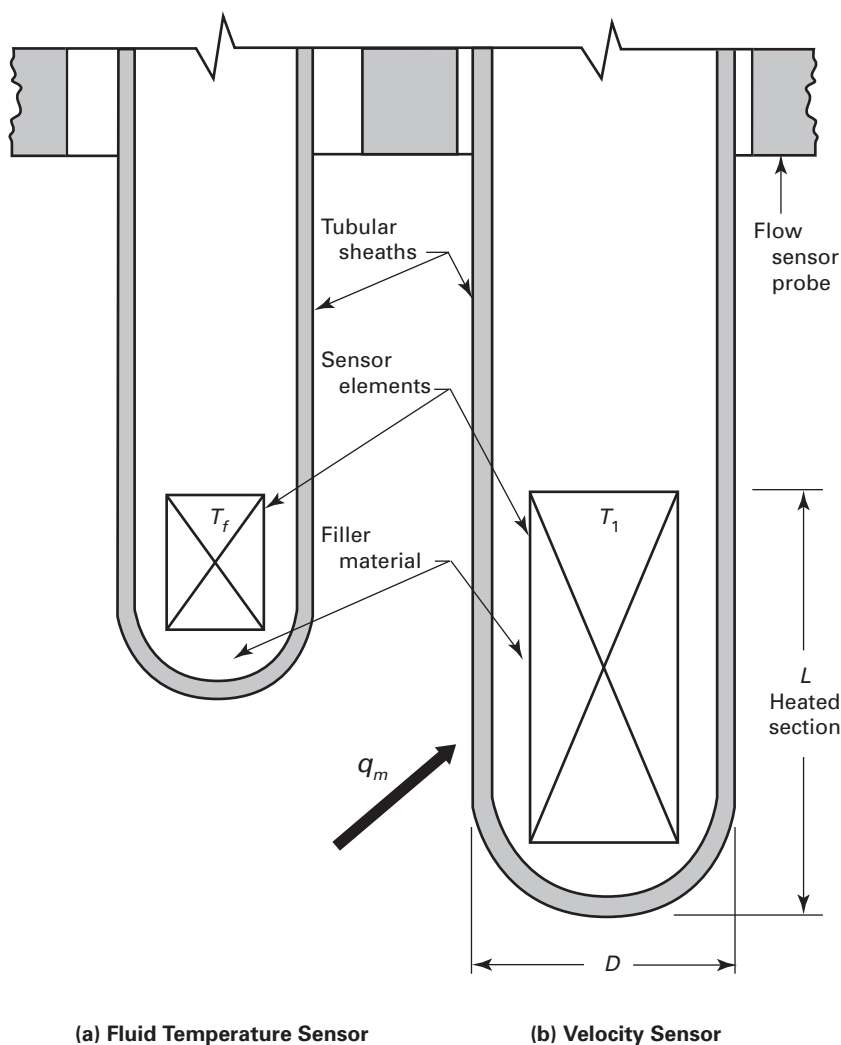Fig. 3.2-1 Flow Sensor of Thermal Dispersion Mass Flowmeters**(a) Fluid Temperature Sensor****(b) Velocity Sensor**

elements. This construction has been used for liquid flow applications.

In operation, the fluid temperature sensor measures the fluid temperature T_f . The sensor drive in the transmitter delivers electrical current to the velocity sensor such that it is self-heated to an average temperature, T_1 , elevated above the fluid temperature. The heat convected from the velocity sensor to the flowing fluid provides measurement of fluid mass flow rate, q_m .

3.3 Transmitter

The transmitter is the electronic system providing the flow sensor drive. The transmitter transforms or linearizes the signals from the sensors into engineering outputs of the variables. The transmitter is housed in an enclosure that conforms to relevant codes, such as hazardous location codes or area classifications.

Digital transmitter electronic systems with digital communication and a digital display facilitate flowmeter diagnostics, validation, calibration adjustment, and reconfiguration. Microcomputer-based digital systems provide correction for changes in fluid temperature and optionally for other influence parameters.

3.4 Temperature Compensation

In the great majority of applications for thermal dispersion mass flowmeters, the process fluid is a gas. Some of the properties of gases influencing convective heat transfer depend on gas temperature. The properties of liquids may also depend on the fluid temperature. For this reason, general-purpose thermal dispersion mass flowmeters should have means for compensating for changes in fluid temperature.

The front end of the flow sensor drive is often an analog Wheatstone bridge circuit. The velocity sensor and the fluid temperature sensor are located on opposite legs of the bridge. This provides analog compensation for changes in fluid temperature. The bridge voltage is a high level output signal in the order of several volts, thereby greatly enhancing the signal-to-noise ratio. The Wheatstone bridge and temperature compensation are thoroughly described in the open literature [6–10].

3.5 Modes of Operation

The flow sensor drive has two modes of operation: the constant temperature differential mode and the constant current mode [6, 8]. Figure 3.3-1 shows typical raw non-linear output signals without signal conditioning for both modes. Equation (4-14) and para. I-2 in Mandatory Appendix I discuss these curves and the need for flow calibration.

3.5.1 Constant Temperature Differential Mode. In this mode of operation, the flow sensor drive maintains at a constant value the difference $\Delta T = T_1 - T_f$ between the temperature of the heated velocity sensor, T_1 , and the fluid temperature, T_f . The output signal is the electrical power, W , supplied to the heated velocity sensor required to keep ΔT constant.

3.5.2 Constant Current Mode. In this mode of operation, the flow sensor drive maintains at a constant value the electrical current, I , supplied to the heated velocity sensor. The output signal is ΔT .

4 PRINCIPLE OF OPERATION

This section describes the principle of operation of thermal dispersion mass flowmeters [6–10]. The flow sensor construction used in this discussion is that most commonly deployed: single-ended tubular velocity and fluid temperature sensors mounted in parallel and adjacent to each other. The velocity sensor element and the fluid sensor element are the platinum RTD elements T_1 RTD and T_f RTD, respectively. This is the flow sensor construction of Figs. 3.1-1, 3.2-1, 3.3-1, and 4-1.

Although this section applies to both gas and liquid flows, it has primary application to gas flows because they constitute the vast majority of installations.

The purpose of this description is to provide a general understanding of the principle of operation. It describes the major factors of influence without the detailed complexities like the solution of differential equations. In practice, all thermal dispersion flowmeters should be flow calibrated, following the procedures in Nonmandatory Appendix A.

4.1 Fluids

4.1.1 Gases. Thermal dispersion flowmeters are ideally suited for the measurement of the mass flow rate

of gases. Their sensitivity is highest at lower flows (0 to 30 normal m/s) and at gas pressures that are in the low to medium range (0.1 bars to 10 bars).

4.1.2 Liquids. Thermal dispersion technology is not well suited for liquid flow applications because at the no flow condition a majority of the heat budget is carried away by the liquid due to its high thermal conductivity relative to that of gases. This reduces measurement sensitivity. To avoid cavitation problems ΔT must be set to a relatively low value. This also reduces sensitivity and increases dependence on small changes in liquid temperature. Application to liquid flows should be limited to cases, such as ultra-low flow applications, where thermal dispersion technology offers advantages over other flowmeter technologies.

4.2 Measurement of Mass Flow Rate

Thermal dispersion mass flowmeters measure the heat convectively transferred from the heated velocity sensor to the gas molecules passing through the viscous boundary layer surrounding the sensor's heated cylindrical surface. Since the molecules bear the mass of the gas, thermal dispersion flowmeters directly measure *mass* flow rate.

4.3 First Law of Thermodynamics

Figure 4-1 shows the first law of thermodynamics applied to the heated section of the velocity sensor.

4.3.1 First Law. With reference to Fig. 4-1, the first law of thermodynamics applied to the entire heated section of the velocity sensor at steady-state conditions is heat (or power) into the heated section equals the heat (or power) out, or

$$W = Q + Q_L \quad (4-1)$$

where

I = current supplied to the T_1 RTD

Q = heat convected away from the heated section by the fluid

Q_L = heat loss from the heated section via conduction down the stem of the velocity sensor (stem conduction) to the ambient environment external to the flow body (see para. 4.3.3)


R_1 = electrical resistance of the T_1 RTD

$W = I^2 R_1$ = electrical power supplied to the T_1 RTD

All terms in eq. (4-1) are in units of watts (W). Radiative heat transfer is ignored because it is relatively small, except in extremely high temperature gas flow applications. The term Q is


$$Q = h_e A_e (T_1 - T_f) \quad (4-2)$$

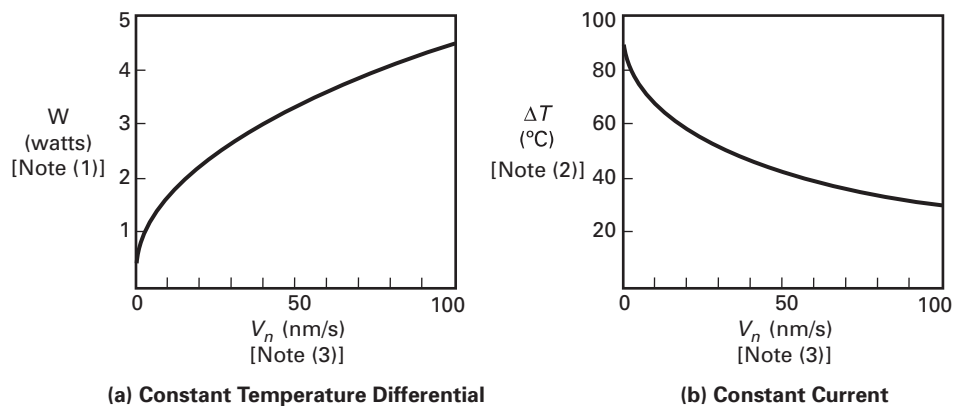

Fig. 3.3-1 Two Modes of Flow Sensor Operation

NOTES:

- (1) $\Delta T = 50^\circ\text{C}$, constant.
- (2) ΔT at zero flow is 50°C .
- (3) V_n is the velocity referenced to "normal" conditions of $T_n = 0^\circ\text{C}$ and $P_n = 101,325 \text{ Pa}$ (1 atm). For air at $T_f = 20^\circ\text{C}$. Curves are approximate.

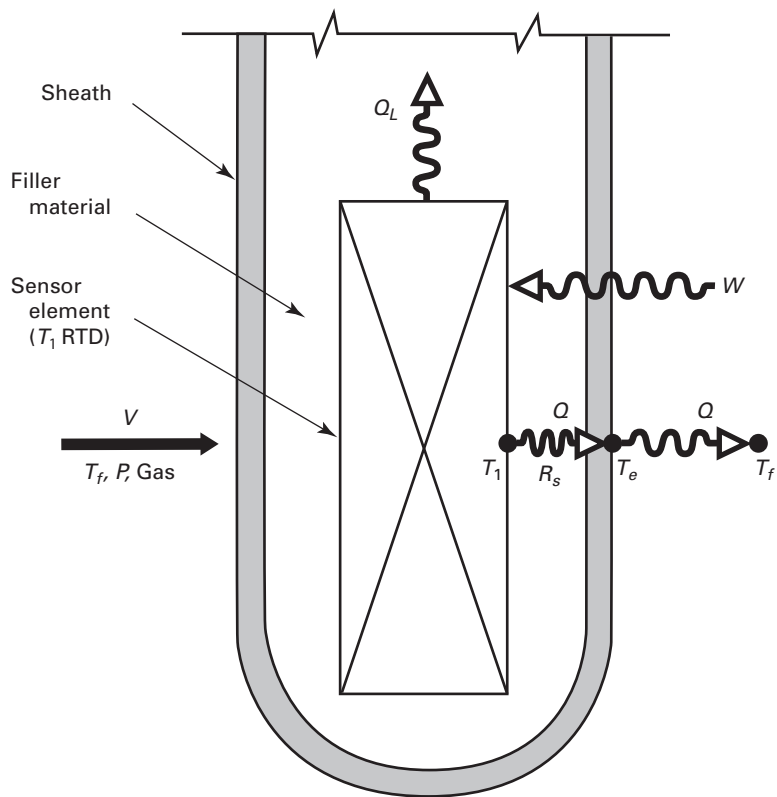Fig. 4-1 Principle of Operation**Heated Section of Velocity Sensor**

where

- $A_e = \pi DL$ = external surface area of the heated section
- D = outside diameter of the velocity sensor
- h_e = "equivalent" film coefficient for convective heat transfer is defined by eq. (4-3)
- L = length of the heated section
- T_1 = average temperature of the T_1 RTD over the length L of the heated section, the quantity directly measured by the T_1 RTD
- T_f = temperature of the flowing fluid measured by the T_f RTD

$$h_e = h / (1 + h A_e R_s) \quad (4-3)$$

where

- h = film coefficient for convective heat transfer from the velocity sensor (h is the quantity we seek)
- R_s = "skin resistance," defined in para. 4.3.2

The final expression for the first law of thermodynamics applied to the entire heated section of the velocity sensor now becomes

$$W = h_e A_e \Delta T + Q_L \quad (4-4)$$

where

$$\Delta T = T_1 - T_f = \text{temperature differential}$$

As discussed in para. 3.5, in the constant temperature differential mode of operation, W is the output quantity, and ΔT is held constant. In the constant current mode of operation, ΔT is the output quantity, and the current, I , is held constant.

4.3.2 Skin Resistance. The average external surface temperature, T_e , over length, L , shown in Fig. 4-1 is less than the temperature T_1 of the T_1 RTD. This is due to a temperature drop that is required to pass the heat Q through the intervening layers of the velocity sensor between the T_1 RTD and the external surface. These intervening layers, the filler material and the tubular sheath, are called the "skin." Their thermal resistance, R_s , is called the "skin resistance." R_s is defined by

$$Q = (T_1 - T_e) / R_s \quad (4-5)$$

At higher flow rates, the skin resistance, R_s , causes the droop, or reduction in sensitivity, of output signals of the flowmeter, as evidenced by Fig. 3.3-1. Skin resistance is an unwanted quantity and should be minimized by manufacturers.

4.3.3 Stem Conduction. Conduction of heat through the stem of the velocity sensor couples the heated section to the ambient environment external to the flowmeter. The value of Q_L in eqs. (4-1) and (4-4) therefore changes with changes in ambient temperature. Stem conduction

is a second unwanted quantity (along with skin resistance) and should be minimized or accounted for by manufacturers.

4.4 Law of Conservation of Mass

The law of conservation of mass (the continuity equation) for the flow conduit or flow body is

$$q_m = \rho V_{ave} A_{pipe} = \rho_b V_{ave, b} A_{pipe} \quad (4-6)$$

where

- A_{pipe} = cross-sectional area of the flow conduit (pipe) or flow body
- $()_b$ = term is referenced to "base" conditions (e.g., "standard" or "normal" conditions) of base temperature, T_b , and base pressure, P_b
- q_m = mass flow rate in the flow conduit or, in the case of in-line flowmeters, the flow body
- V_{ave} = average fluid velocity over A_{pipe}
- ρ = mass density of the fluid

From eq. (4-6) it is obvious that $\rho V_{ave} = \rho_b V_{ave, b}$. Likewise, continuity considerations require the same relationship for the point velocity, V ; i.e.

$$\rho V = \rho_b V_b \quad (4-7)$$

The flow sensor measures the point velocity at a point (or small volume) within the conduit's cross-sectional area, A_{pipe} . The ratio, F_c , of the average velocity, V_{ave} , to the point velocity, V , is defined as

$$F_c = V_{ave} / V = \text{conduit factor} \quad (4-8)$$

In-line thermal dispersion mass flowmeters with a built-in flow conditioner have a conduit factor, F_c , close to unity, as do insertion meters in undisturbed flow downstream of nozzles or smooth contractions. Most insertion flowmeters have the center of the active area of the velocity sensor located at the conduit's centerline. For this case and with a fully developed velocity distribution in the conduit, reference [11] presents a curve of F_c as a function of the Reynolds number, Re_{pipe} , of the conduit and wall roughness. Typical values of F_c from this curve are

$$\begin{aligned} F_c &= 0.5 \text{ for } Re_{pipe} \leq 2,000 \\ F_c &= 0.83 \pm 0.03 \text{ for } Re_{pipe} \geq 40,000 \end{aligned}$$

Some manufacturers provide correlations for F_c over the range of Re_{pipe} between 0 and 10^6 .

4.5 Correlations for Convective Heat Transfer

4.5.1 General Empirical Correlation. The film coefficient, h , is found using empirical correlations. In most applications the fluid is a gas; compressibility effects are negligible; and the gas pressure is not excessively high.



In this case, the correlation for h is expressed as a function of the following nondimensional parameters.

$$Nu = f(Re, Pr) \quad (4-9)$$

where

- c_p = coefficient of specific heat of the fluid at constant pressure
- k_f = thermal conductivity of the fluid
- $Nu = hD/k_f$ = Nusselt number, the nondimensional heat-transfer parameter
- $Pr = \mu c_p / k_f$ = Prandtl number, the ratio of the diffusivity of momentum to the diffusivity of heat (a fluid properties parameter)
- $Re = \rho V D / \mu$ = Reynolds number of the velocity sensor, the nondimensional ratio of dynamic to viscous forces, based on D
- μ = absolute viscosity of the fluid

4.5.2 Example Correlations. Following are two examples of empirical correlations.

$$Nu = b_1 + b_2 Pr^{b_3} Re^{b_4} \quad (4-10)$$

$$Nu = Pr^{b_1} (b_2 Re^{b_3} + b_4 Re^{b_5}) \quad (4-11)$$

where

b_i = gas factors

The gas factors in the above equations are constants found via flow calibration by the manufacturer following the procedures in Nonmandatory Appendix A.

4.6 Solution for Reynolds Number, Re

4.6.1 General Solution. The primary desired output variable is the fluid mass flow rate q_m flowing through the conduit or flow body. Q_m depends on the product ρV , the fluid's mass density times the point velocity, embodied in the Reynolds number $Re = \rho V D / \mu$. ρV is often called the "mass velocity" and is the mass flow rate per unit area ($\text{kg/s} \cdot \text{m}^2$). The solutions for the output variables presented in para. 4.7 are proportional to the Reynolds number, Re . In this section we find Re as a function of the Nusselt number.

Nu is found by combining eqs. (4-3) and (4-4).

$$\begin{aligned} Nu &= hD/k_f \\ &= [D/(k_f A_e)] [W - Q_L] / [\Delta T - (W - Q_L) R_s] \end{aligned} \quad (4-12)$$

The terms D , A_e , and R_s in eq. (4-12) are either directly or indirectly determined by the manufacturer via flow calibration for each flowmeter following the procedures in Mandatory Appendix I.

The solution for Nu is inserted into the empirical correlation eq. (4-9) [e.g., eqs. (4-10) and (4-11)] that is then solved for Re .

4.6.2 Example Solution. For example, if the correlation in eq. (4-10) is used, Re can be found explicitly as

$$Re = [(Nu - b_1) / (b_2 Pr^{b_3})]^{(1/b_4)} \quad (4-13)$$

Insertion of the expression for Nu given by eq. (4-12) into the above equation yields the desired solution for Re for this example.

$$Re = \left[\frac{\left[\frac{D}{K_f A_e} \times (W - Q_L) \right] / \left[\Delta T - (W - Q_L) R_s \right] - b_1}{b_2 Pr^{b_3}} \right]^{(1/b_4)} \quad (4-14)$$

4.7 Solutions for Output Variables

4.7.1 Purpose. This section presents final closed-form expressions for all output variables of thermal dispersion mass flowmeters based on the results of previous paras. 4.3 through 4.6.

In-line flowmeters are flow calibrated (see Mandatory Appendix I) to directly measure the fluid flow rate in the pipeline and thereby measure the flow rate quantities q_m , $q_{v,r}$, and $q_{v,b}$ in eqs. (4-15), (4-16), and (4-17), respectively.

Insertion flowmeters are often flow calibrated (see Mandatory Appendix I) to directly measure the entire flow rate in a flow conduit and thereby measure the flow rate quantities q_m , $q_{v,r}$, and $q_{v,b}$ in eqs. (4-15), (4-16), and (4-17), respectively. Alternatively, insertion flowmeters are flow calibrated to measure the velocity at a point in the conduit's cross-sectional area and thereby directly measure the quantities V and V_b in eqs. (4-18) and (4-19), respectively, and indirectly measure the flow rate quantities q_m , $q_{v,r}$, and $q_{v,b}$ by applying the appropriate conduit factor F_c in eqs. (4-15), (4-16), and (4-17), respectively.

4.7.2 Other Approaches. The following closed-form expressions and their derivations are presented solely to describe the principle of operation of thermal dispersion mass flowmeters. They are primarily relevant to digital flowmeters. Some manufacturers may use other approaches, particularly those with analog or hybrid analog/digital products.

4.7.3 Definitions of Terms Used in Solutions for Output Variables

A_{pipe} = cross-sectional area of flow conduit or flow body

D = outside diameter of the velocity sensor

F_c = conduit factor, the flow profile correction factor [see eq. (4-8)]

$Re = \rho V D / \mu$ = Reynolds number of the velocity sensor, based on D

μ = absolute viscosity of the fluid

ρ = mass density of the fluid



$()_b$ = subscript signifying term is referenced to "base" conditions of fluid temperature T_b and fluid pressure P_b , for example:

(a) For "standard" ("s") base conditions:
 $T_b = 21.1^\circ\text{C}$ (or 70°F); $P_b = 101,325$ Pa (1 atm)

(b) For "normal" ("n") base conditions:
 $T_b = 0^\circ\text{C}$; $P_b = 101,325$ Pa (1 atm)

4.7.4 Mass Flow Rate in a Flow Conduit, q_m (kg/s)

$$q_m = (F_c A_{\text{pipe}})(\mu/D) Re \quad (4-15)$$

4.7.5 Volumetric Flow Rate in a Flow Conduit, q_v (m^3/s)

$$q_v = (F_c A_{\text{pipe}}/\rho) (\mu/D) Re \quad (4-16)$$

4.7.6 Volumetric Flow Rate in Flow Conduit Referenced to Base Conditions, $q_{v,b}$ (bm^3/s)

$$q_{v,b} = (F_c A_{\text{pipe}}/\rho_b) (\mu/D) Re \quad (4-17)$$

(a) For "standard" base conditions, "b" = "s."

(b) For "normal" base conditions, "b" = "normal."

4.7.7 Point Velocity, V (m/s)

$$V = (1/\rho) (\mu/D) Re \quad (4-18)$$

4.7.8 Point Velocity Referenced to Base Conditions, V_b (bm/s)

$$V_b = (1/\rho_b) (\mu/D) Re \quad (4-19)$$

(a) For "standard" base conditions, "b" = "s."

(b) For "normal" base conditions, "b" = "normal."

4.7.9 Mass Flow Rate in a Flow Conduit Measured Via a Multipoint Insertion Flowmeter, q_m (kg/s). In flow conduits with large cross-sectional areas, the mass flow rate, q_m , through the entire conduit is often measured with a multipoint insertion thermal dispersion mass flowmeter, especially if the measurement plane is downstream of an elbow or other upstream flow disturbances [5]. Multipoint insertion flowmeters are designed and installed such that a separate flow sensor is located at the centroid of N equal areas in the cross-sectional area, A_{pipe} , of the conduit. q_m is found as follows:

$$q_m = q_{m,1} + q_{m,2} + \dots + q_{m,N} \quad (4-20)$$

where

$q_{m,i} = (A_{\text{pipe}}/N) (\mu/D) Re_i$ = mass flow rate measured by flow sensor i ($i = 1, 2, \dots, N$)

4.7.10 Gas Mass Density, ρ (kg/m^3). The mass density for gases obeying a modified perfect-gas-law equation of state is calculated as follows:

$$\rho = PM / (Z R T) \quad (4-21)$$

where

M = molecular weight of the gas

P = absolute static pressure of the gas

R = the universal gas constant

T = absolute static temperature of the gas

Z = compressibility of the gas

The gas temperature, T , in eq. (4-21) either is directly measured by flowmeters with the multivariable feature or is inputted from a nearby temperature transducer in the pipeline. The gas pressure, P , is inputted from a nearby pressure transducer in the pipeline.

5 GUIDELINES FOR FLOWMETER SELECTION

Improper flowmeter selection is a common factor that can impair flowmeter performance in the field.

This section is primarily applicable to gas flow applications. Paragraph 6.2.2 describes liquid flow applications. The guidelines presented in this section are valid for the most common, or typical, thermal dispersion mass flowmeters. It is understood that departures from the statements and numerical values herein may exist for some manufacturers.

The following information is used to select and size both in-line and insertion flowmeters:

- gas composition
- mass flow rate range
- pressure range
- temperature range
- permanent pressure loss
- performance (accuracy, repeatability, time response, and reproducibility)

Most manufacturers use sophisticated software accounting for these variables to properly select and size the flow rate for the user's application. It is recommended that the user rely on the veracity of the flowmeter selected via this process.

Table A-1 in Nonmandatory Appendix A presents a typical table used for sizing in-line flowmeters for air flow applications.

The specifications in the following may vary from manufacturer to manufacturer. Users should not deploy thermal dispersion mass flowmeters in applications not falling within the manufacturer's specifications. Non-conforming applications may require that the manufacturer provide a special flowmeter design or flow calibration.

5.1 Mass Flow Rate Range

Mass flow rate ranges are expressed here as the point mass velocity, V_b , referred to base conditions of T_b and P_b . V_b is explicitly applicable to insertion flowmeters. The mass flow rate, q_m , for in-line flowmeters is found via eq. (4-6) and by multiplying V_b by $F_c \rho_b A_{\text{pipe}}$.



5.1.1 Minimum Mass Flow. The flowmeter's accuracy specification should be taken into account in determining the minimum mass flow rate. Thermal dispersion mass flowmeters are in the category of flowmeters that do measure zero flow. Detectable minimum point mass velocities as low as approximately 20 sfpm (approx. 0.1 normal m/s) are specified by some manufacturers.

5.1.2 Maximum Mass Flow Rate. The following limitations should be considered in determining the maximum mass flow rate:

(a) The Mach number (the ratio of the actual velocity to the speed of sound of the gas) should not exceed approximately 0.3 to avoid unwanted compressibility effects.

(b) Measurement sensitivity should be sufficiently high. Figure 3.3-1 shows the decrease in measurement sensitivity at higher mass flow rates.

(c) The permanent pressure loss should not be excessive. Typically permanent pressure loss is sufficiently low that it is not a consideration (see para. 5.4 and Nonmandatory Appendix A).

For both in-line and insertion flowmeters the typical maximum point mass velocity for air referenced to base conditions is approximately 20,000 sfpm (approximately 100 normal m/s). With special flow calibration, the maximum point mass velocity can be extended to approximately 35,000 sfpm (approximately 175 normal m/s). Nonmandatory Appendix A shows typical maximum air mass flow rates through in-line flowmeters of various sizes.

5.1.3 Rangeability. Rangeability is the ratio of the maximum mass flow rate to the minimum flow rate. Thermal dispersion mass flowmeters are in a class of flowmeters that have high rangeability. Typical flow calibration yields rangeabilities from 10:1 to 100:1.

Manufacturers extend the mass flow rate range of thermal dispersion mass flowmeters by dividing the total range into separate segments that are then individually flow calibrated. In this case, manufacturers should use multiple flow calibration standards if required to ensure specified accuracy. Multirange flow calibration can yield rangeabilities exceeding 100:1.

5.2 Pressure Range

The process pressure range of both in-line and insertion meters depends on the pressure rating of the process connection. For in-line flowmeters with Class 150 lb flanges (PN 16), the typical process pressure range specified by manufacturers is 0 psig to 230 psig (0 barg to 16 barg) at ambient temperature. The maximum pressure typically specified for in-line flowmeters is 300 psig (approximately 20 barg) at ambient temperature and requires threaded or 300 ANSI/PN 40 flanges. For insertion flowmeters with a compression fitting process connection, the maximum pressure rating typically

specified is 500 psig (approximately 35 barg) at ambient temperature. A typically specified minimum pressure is -7 psig (approximately -0.5 barg) for both in-line and insertion flowmeters.

Because the strength of materials degrades with increasing temperature, for safety purposes users are cautioned to follow the manufacturer's specifications for maximum process pressure versus process temperature.

5.3 Temperature Range

Process temperature ranges specified by manufacturers typically range from approximately 15°F to 250°F (approximately -10°C to 120°C) to -40°F to 350°F (approximately -40°C to 175°C). Some manufacturers offer optional temperature upper limits ranging from 750°F to 930°F (approximately 400°C to 500°C).

5.4 Permanent Pressure Loss

Thermal dispersion mass flowmeters are in the category of flowmeters with relatively low permanent pressure loss. In-line flowmeters, without a flow conditioner, have negligible permanent pressure loss; insertion flowmeters having flow conduits with internal diameters equal to, or larger than, approximately 3 in. (approximately 0.1 m) have negligible permanent pressure loss. Nonmandatory Appendix A shows the permanent pressure loss of typical in-line flowmeters.

5.5 Gas Composition

Thermal dispersion mass flowmeters should be used for pure gases or gas mixtures of known composition. Typical pure gases include nitrogen, oxygen, carbon dioxide, methane, propane, hydrogen, argon, and helium. Typical gas mixtures include air, natural gas, combustion gases, stack gases, flare gases, and digester gases.

Consideration should be given to water vapor content and the potential for condensation of gas components. The gas should be compatible with, and not corrode, the wetted materials of the flowmeter.

5.6 Performance

5.6.1 Mass Flow Rate Measurement Accuracy and Repeatability. Manufacturers of thermal dispersion mass flowmeters should include the combined effects of linearity, repeatability, hysteresis, and zero stability in their mass flow rate accuracy specification. This topic is discussed further in para. 6.1.6, Influence Parameters.

Manufacturers typically present the overall accuracy, A_t , (in units of percent of reading) in the following ways:

(a) based on percent of reading A_r ,

$$A_t = \pm A_r \quad (5-1)$$

(b) based on percent of full scale A_{fs}

$$A_t = \pm A_{fs} q_{mfs} / q_m \quad (5-2)$$



(c) combination of the above

$$A_t = \pm (A_r + A_{fs} q_{m,fs} / q_m) \quad (5-3)$$

where

q_m = actual mass flow rate

$q_{m,fs}$ = full scale (upper range limit) mass flow rate of flowmeter

Manufacturers should express the overall accuracy, A_t , in terms of the specific ranges of the reference conditions of mass flow rate, process temperature, and process pressure for which it applies. The manufacturer should provide additional accuracy terms covering the case where the actual process temperature, T_p , and pressure, P , fall outside of their reference condition ranges.

Typically, these terms are presented as a temperature influence coefficient, C_T , and a pressure influence coefficient, C_P . C_T is in units of percent of reading accuracy per degree centigrade, or equivalent. C_P is in units of percent of reading accuracy per bar, or equivalent. These influence coefficients are multiplied respectively by the absolute value of the difference between the actual temperature or pressure and the upper or lower limits of the temperature or pressure reference condition ranges, and are then added to the relevant overall accuracy statement in eqs. (5-1), (5-2), or (5-3). This is better explained by the Example of Accuracy Calculation in Nonmandatory Appendix B.

Repeatability, expressed by the manufacturer as a percentage of reading or of full scale, may also be important in flowmeter selection. Typical manufacturers' repeatability specifications fall in the range of 0.1% to 0.5% of reading.

5.6.2 Multivariable Measurement Accuracy. Manufacturers of thermal dispersion mass flowmeters with optional temperature measurement typically express temperature measurement accuracy as an error in degrees Centigrade ($^{\circ}\text{C}$). Manufacturers should express the overall accuracy in terms of the specific range of temperature to which it applies and provide a temperature influence coefficient, or the equivalent, covering departures from this range.

5.6.3 Time Response. Manufacturers' specified time response to a change in mass flow rate ranges from approximately 1 sec to 7 sec to within $\pm 63\%$ of the final value (i.e., one time constant) for flowmeters operated in the constant temperature differential mode and for flowmeters operated in the constant current mode (para. 3.5) ranges from approximately 7 sec to 15 sec to within $\pm 63\%$ of the final value. Constant current operation is slower than constant temperature differential operation because the temperature of the entire mass of the velocity sensor must change if velocity changes. Time response becomes faster as the mass flow rate increases. Most manufacturers specify time response at the maximum mass flow rate of their flowmeter. Users should

select flowmeters that use the constant temperature differential mode of operation for applications requiring faster time response.

5.6.4 Reproducibility. The reproducibility, or stability over time, of the flow sensor depends on its exposure to severe operating conditions, such as temperature cycling, temperature over ranging, and pipeline vibrations. Velocity sensors constructed with filler materials such as ceramic cements or epoxies that are exposed to such severe operating conditions may be susceptible to long-term drift (see para. 3.2). Velocity sensors that avoid the use of these materials minimize the effect of long-term drift when subjected to severe operating conditions. Preferably, susceptible flowmeters should not be installed at locations in the pipeline that have deleterious operating conditions. If this is not possible, devices that reduce the severity of the operating conditions should be installed upstream of the flowmeter.

6 GUIDELINES FOR INSTALLATION AND APPLICATIONS

Suboptimal performance of thermal dispersion mass flowmeters is often caused by installation effects and misapplications.

Flowmeter installation should take into account physical constraints, flow conditions (including minimum and maximum fluid densities), application considerations, and safety [11, 12]. The manufacturer should specify installation dimensions, preferred installation configurations, and any installation constraints or restrictions of use.

6.1 Installation

6.1.1 General Installation Criteria

(a) With the exception of hot-tap applications (see para. 8.7), during installation the process flow and electrical power should be turned off, the line should not be pressurized, and the line's temperature should not be excessive.

(b) The flowmeter should be installed such that the direction of flow in the pipe coincides with flow direction arrow or indicator on the flowmeter.

(c) The process pressure and temperature must not exceed the manufacturer's specified ratings.

(d) The class and type of pipe, process connections, pipe materials, and erosion, corrosion, and deposition of material in the pipeline should be considered.

(e) The flowmeter's process connections should be

(1) seated squarely on the mating fluid connection seals such that no part of the gasket is in the flow

(2) secured following the manufacturer's guidelines such that the allowable leak-rate specifications are satisfied



(f) Any applicable hazardous area classification must be considered. The cable entry into the transmitter enclosure shall meet the hazardous area standard.

(g) Proper wiring and electrical power should be verified and follow applicable safety codes. The voltage, its frequency, and its polarity should meet the manufacturer's specifications.

(h) The environmental effects on the flowmeter, such as ambient temperature, ambient pressure, humidity, corrosive atmospheres, mechanical shock, mechanical pipeline vibrations, and external electromagnetic fields should be considered. High ambient and process temperatures may require the installation of remote electronics (see para. 6.1.5).

(i) Shut-off valves upstream and downstream of the flowmeter (installed for the purpose of isolating, removing, zeroing, or flow calibrating the flowmeter) should not disturb the main process flow when not in use.

(j) Thermal dispersion mass flowmeters do operate in pulsating flows, but performance may be degraded in intense pulsating flows, such as locations immediately downstream of pumps. In this case, isolation or pulsation damping devices should be considered. The manufacturer's recommendations should be observed regarding the use of such devices.

6.1.2 Spatial and Orientation Requirements

(a) Sufficient spatial clearance should be provided for flowmeter installation. Special considerations should take into account the need for safe and convenient human access, as well as space for in situ flow calibration, if required.

(b) Sufficient clearance should be provided for insertion flowmeters to facilitate their unobstructed removal.

(c) Insertion flowmeters with hot-tap hardware should have extra clearance, and the proper insertion depth should be verified.

(d) The flowmeter should not be installed at a location in the piping system that is susceptible to liquid collection or condensation.

(e) The flowmeter should be oriented in the flow conduit, or pipe, in the orientation for which it was flow calibrated. This is important because the zero flow reading depends on natural convection which in turn depends on the orientation of the flow sensor relative to the gravitational force vector.

(f) The most common deployment is in horizontal pipes. In this case, the de facto flowmeter orientation is with the flowmeter mounted on top of the pipe.

(g) For deployment in vertical pipes, the flow direction either upward or downward should be specified by the user.

6.1.3 Process Fluid Quality. For gas applications, the use of filters, traps, or other protective devices may be required for removing solids, liquids, and liquid drops that could cause damage to the flow sensor or

induce errors in measurement. In general, these devices should be placed upstream of the flowmeter. Occasional liquid drops striking the heated velocity sensor usually do not cause damage, but will cause a spike in output until they burn off.

For liquid applications (see para. 6.2.2), the use of strainers, filters, air and vapor eliminators, or any other protective devices may be required to remove solids, vapors, and gas bubbles that could cause damage to the flow sensor or induce errors in measurement. These devices are placed upstream of the flowmeter.

6.1.4 Flow Conditions and Straight Pipe Length Requirements.

The performance of thermal dispersion mass flowmeters can be degraded if the flowmeter is installed where flow conditions are different from those for which the flowmeter was calibrated. Components in the pipe system upstream and to a lesser extent downstream of the flowmeter can create flow profile nonuniformities, swirling flow, and turbulence that may degrade flowmeter performance. Such flow-disturbing components include single or multiple elbows, expansions, contractions, tees, heaters, coolers, valves, etc. The flowmeter's location should be chosen to minimize the effect of such flow disturbances. It is preferred that control valves be installed downstream of the flowmeter.

Viscous forces in a length of straight pipe before and after the flowmeter tend to reduce flow nonuniformities, and create a fully developed flow profile with sufficiently long length. To ensure specified performance and avoid installation effects, the manufacturer's recommended straight pipe lengths upstream and downstream of the flowmeter should be followed. The straight pipe requirements for typical in-line and insertion flowmeters are shown in Tables 6.1.4-1 and 6.1.4-2, respectively.

Flow conditioners installed as separate units upstream of in-line and insertion flowmeters may be used to reduce the effect of upstream flow-disturbing components. Alternatively, an in-line flowmeter with a built-in flow conditioner may be used.

6.1.5 Remote Electronics Installation. If the ambient temperature exceeds the manufacturer's specified limits, the electronics transmitter enclosure should be mounted remotely. A typical upper-limit value is 140°F (approximately 60°C). In excessively hot conditions, consideration should be given to installing the flowmeter horizontally so that natural convection carries less heat from the hot pipeline to the transmitter enclosure.

For remote installation, the cable connecting the transmitter enclosure to the flow sensor should be that provided by the manufacturer and typically should not be lengthened or shortened by the user because the electrical resistance of the cable is part of the flow sensor's circuit. Some manufacturers provide compensation for cable length.



Table 6.1.4-1 Straight Pipe Length Requirements for an In-Line Flowmeter With a Built-In Flow Conditioner

Flow Disturbing Component	Thermal Dispersion Mass Flowmeter [Note (1)]		Orifice Plate [Note (4)] (Upstream Length)
	Upstream [Note (2)]	Downstream [Note (3)]	
Single 90-deg elbow	1 D	0 D	28 D
Reduction (4:1)	3 D	0 D	14 D
Expansion (4:1)	3 D	0 D	30 D
After control valve [Note (5)] or pressure regulator	3 D	0 D	32 D
Two 90-deg elbows in same plane	3 D	0 D	36 D
Two 90-deg elbows in different planes	5 D	0 D	62 D

GENERAL NOTES:

- (a) Straight pipe length requirements at 1 bara pressure. Consult manufacturer for pressure effects.
 (b) These specifications may vary from manufacturer to manufacturer. Consult the manufacturer.

NOTES:

- (1) For an in-line flowmeter with a flow conditioner consisting of two separated perforated plates located in the flow body upstream of the flow sensor.
 (2) Number of diameters D of straight pipe required between the exit of the upstream flow disturbing component and the entrance of the flowmeter.
 (3) Number of diameters D of straight pipe required between the exit of the flowmeter and the entrance of the downstream flow disturbing component.
 (4) For comparison purposes only. The table shows the number of diameters D of upstream straight pipe required between the exit of the upstream flow disturbing component and an ISO Standard 5167 orifice plate with a beta ratio of 0.7.
 (5) If the valve is always wide open, base the length requirement on the valve's inlet or outlet fitting.

Table 6.1.4-2 Straight Pipe Length Requirements for Insertion Flowmeters With No Flow Conditioning

Flow Disturbing Component	Upstream [Note (1)]	Downstream [Note (2)]
Single 90-deg elbow	15 D	5 D
Reduction	15 D	5 D
Expansion	30 D	10 D
After control valve [Note (3)] or pressure regulator	40 D	5 D
Two 90-deg elbows in same plane	20 D	5 D
Two 90-deg elbows in different planes [Note (4)]	40 D	10 D

GENERAL NOTES:

- (a) Straight pipe length requirements at 1 bara pressure. Consult manufacturer for pressure effects.
 (b) These specifications may vary from manufacturer to manufacturer. Consult the manufacturer.

NOTES:

- (1) Number of diameters D of straight pipe required between the exit of the upstream flow disturbing component and the insertion flowmeter.
 (2) Number of diameters D of straight pipe required between the insertion flowmeter and the entrance of the downstream flow disturbing component.
 (3) If the valve is always wide open, the length requirement should be based on the valve's inlet or outlet fitting.
 (4) For three 90-deg elbows, the required length should be doubled.



6.1.6 Influence Parameters. Process temperature and pressure and ambient temperature have a secondary influence on mass flow rate measurement accuracy. Very low process density may affect some manufacturers' flowmeter performance. To achieve best measurement accuracy, users should have knowledge of the actual process temperature and pressure and ambient temperature of their application and specify those conditions to the vendor before procuring the flowmeter. For best measurement accuracy, the manufacturer should match these conditions during flow calibration.

6.1.6.1 Process Temperature. As described in para. 3.4, accurate measurement requires that the flowmeter have means for compensating for changes in process temperature, either via analog, digital, or combined analog and digital temperature compensation. The temperature influence coefficient, C_T , described in para. 5.6.1 accounts for the effect of process temperature on the overall accuracy of mass flow rate measurement. Better temperature compensation leads to lower values of C_T .

6.1.6.2 Process Pressure. Thermal dispersion mass flowmeters intrinsically correct for the majority of changes in process pressure because they directly measure the Reynolds number. The Reynolds number depends on the gas mass density which, in turn, depends on the pressure. Nevertheless, this correction does not account for the relatively weak effect of process pressure on natural convection that primarily influences the zero and lower flow ranges. The pressure influence coefficient, C_P , described in para. 5.6.1 accounts for the effect of process pressure on the overall accuracy of mass flow rate measurement. In the event that the actual process pressure in the field is different from that at flow calibration, some flowmeters with digital electronics provide pressure compensation by facilitating the user inputting the actual line pressure measured by a separate pressure transducer located nearby in the process line.

6.1.6.3 Ambient Temperature. The stem conduction phenomenon described in para. 4.3.3 couples the flow sensor with the ambient temperature external to the flowmeter. If the actual ambient temperature in the field is different from that at flow calibration, stem conduction can degrade measurement accuracy. This influence is worse in lower flow ranges and in flowmeters with high stem conductance, i.e., those with relatively short velocity and temperature sensors. Some flowmeters with digital electronics provide compensation for changes in ambient temperature.

6.2 Applications

6.2.1 Gas Flow Applications. The vast majority of applications are gas flow applications because they benefit from a high sensitivity of measurement (see para. 4.1.1). All previous subsections in this section 6 are primarily devoted to gas flow applications.

6.2.2 Liquid Flow Applications. Liquid flow applications are a minor fraction of the applications for thermal dispersion mass flowmeters. The diminished sensitivity of liquid flow applications is discussed in para. 4.1.2.

The following should be considered in liquid flow applications. In all cases manufacturers' specifications should be followed:

(a) The difference ΔT between the temperature of the heated velocity sensor and the temperature of the liquid shall not exceed an upper critical limit. For water flows, this critical limit is approximately 10°C to 20°C. If the critical limit is exceeded, higher liquid flows may reduce the pressure behind the heated velocity sensor to the extent that flashing to the vapor phase and subsequent cavitation may occur. This phenomena can cause erratic and erroneous measurements as well as damage to the flow sensor. Flow sensors operated in the constant temperature differential mode are preferred for liquid flow applications because ΔT is instantaneously maintained at its constant value preselected for the liquid flow applications (see para. 3.5.1). Flow sensors operated in the constant current mode have a variable temperature difference that is difficult to set up for liquid flow (see para. 3.5.2).

(b) The process liquid should meet the fluid quality standards set forth in para. 6.1.3. Industrial liquid flows with poor fluid quality can cause contamination and fouling of the flow sensor.

6.3 Zero and Span Adjustment

After flowmeter installation is complete, a zero adjustment following the manufacturer's instructions may be needed if the zero offset is unacceptable. To properly check or adjust the zero, the flow must be stopped. It is recommended that both upstream and downstream valves are closed during the process of zero adjustment. If possible, zero adjustment should be made under actual temperature and pressure process conditions.

After installation, a span adjustment can be made if needed, following the manufacturer's instructions. Electrical span and multiple-point flow calibration verification and adjustment can be accomplished by using an accurate external digital voltmeter. Nevertheless, only a flow calibration using a flow calibration standard in series with the flowmeter can be used with absolute certainty to span and calibrate the flowmeter. This is achieved either in situ or by sending the flowmeter to the factory or a certified flow facility for flow recalibration. The flow calibration entity should follow the guidelines set forth in Nonmandatory Appendix A.

Before making field adjustments, the user should verify that the flowmeter is not actively monitoring or reporting to any master control system. Adjustments to the electronics may cause direct changes to flow settings.



7 INSPECTION AND COMPLIANCE

If applicable, and upon request, the manufacturer should provide the following certifications to the user:

- (a) material certificates for pressure-containing parts
- (b) certificate of conformance with applicable hazardous area classifications
- (c) flow calibration certificate and performance results
- (d) certificate of suitability for sanitary applications, if applicable

Since the flowmeter is an integral part of the piping system, it may be subjected to special inspection test procedures similar to those applicable to other pipeline equipment or instrumentation. This could include a dimensional check, hydrostatic test, and radiographic and/or ultrasonic tests to verify weld integrity. Upon request, manufacturers performing these special tests should make the results available to the user as a certified report.

8 SAFETY

Thermal dispersion mass flowmeters may be used in high pressure and high temperature applications. They also may be used for flammable and toxic gas applications and may be installed in locations with external flammable atmospheres. Therefore, care must be taken to ensure that the integrity of the flowmeter and general safety is maintained under actual process conditions.

8.1 Manufacturers' Specifications

Flowmeters shall not be used in conditions that fall outside the manufacturer's specifications, irrespective of whether they are the manufacturer's normal published specifications or those resulting from a special request. The following issues must be given consideration in providing for the safety and protection of users and their property.

8.2 Process Pressure and Temperature

8.2.1 Design and Construction. For obvious reasons, a burst or major leak in the flowmeter must be avoided. Manufacturers should design and construct their flowmeters taking this into consideration. During operation, users shall avoid overpressurizing and overheating the flowmeter.

The degradation in the strength of materials with increasing process temperature should be taken into account. Manufacturers shall express the pressure ratings of their flowmeters in terms of the intended temperature range of operation and should properly convey the information that the upper-limit pressure rating decreases as process temperature increases.

8.2.2 Pressure Testing. Manufacturers should hydrostatically test the fully assembled wetted parts

of their flowmeters. Upon request, manufacturers shall provide evidence confirming that the fully assembled flowmeter was tested. This evidence shall be available in terms of either a certificate or a test procedure.

8.3 Hazardous Area Locations

If the flowmeter is located in a hazardous area, it shall comply with applicable codes and standards. Explosion proof transmitter enclosures shall comply with applicable standards. Upon request, the manufacturer shall provide the user with a certificate indicating that the flowmeter is in conformance with the applicable standards. The user shall install and operate the flowmeter in accordance with the applicable standards.

8.4 Electrical Safety

During installation of the flowmeter, the user shall perform the electrical wiring with the power off. Special caution shall be exercised to avoid shocks when wiring the flowmeter to AC power. Manufacturers' instructions and applicable electrical safety and fire prevention codes shall be followed.

If applicable, the flowmeter should have the appropriate certification ensuring that electromagnetic fields generated by the flowmeter do not interfere with proximal electrical devices, and vice versa.

8.5 Leaks

Thermal dispersion mass flowmeters may be used with unhealthful or irritating gases. Manufacturers should publish the leak rates of the flow bodies of their flowmeters and, upon request, provide the user with a leak test certificate or a test procedure. It is recommended that the user make certain that the flowmeter is properly installed and seated squarely on its seals to minimize process gas leaks. Seals should be inspected to ensure their integrity prior to installation.

8.6 Fluid Quality

8.6.1 Erosion. The effect of possible erosion of the flow body depends on the gas velocity and the concentration, size, and composition of solid, and to a lesser extent, liquid particles suspended in the flow. Although typically of minor concern in gas flow applications, erosion should be assessed for each type of use of the flowmeter.

In liquid flows, cavitation and suspended solid particles that may cause erosion should be assessed.

8.6.2 Corrosion. The flowmeter selected should be constructed of materials that are compatible with the fluid. Special attention should be given to corrosive gases or liquids. When in its liquid or droplet form, liquids can react with gases to form acids or other corrosive agents. Such foreign components should be eliminated from the pipeline via upstream traps or other filtering devices.



8.6.3 Unsafe Flow Calibration Gases. As shown in Mandatory Appendix I, the flow-calibrating entity should provide proper venting of unsafe flow calibration gases, such as toxic or corrosive gases. Additionally, it is recommended that the flow calibration system be thoroughly purged with an inert gas.

8.7 Hot Tapping

In some applications, insertion flowmeters are installed in the pipeline with hot-tap hardware. The hot-tap assembly provides an isolation valve facilitating withdrawal and removal of the insertion flowmeter from an active pipeline without interruption of the flow or leakage of fluid. The pressure rating of the hot-tap hardware should meet, or exceed, that of the pipeline. For safety purposes, hot tapping should be performed by a trained professional, and the installation should be done with caution. Governmental regulations often require a hot-tap permit. The user is responsible for providing proof of such a permit.

9 REFERENCES

9.1 General References

The following is a list of publications referenced in this Standard.

ASME B31.3, Process Piping

ASME MFC-21.1, Measurement of Fluid Flow by Means of Capillary Tube Thermal Mass Flowmeters and Controllers

Publisher: The American Society of Mechanical Engineers (ASME), Three Park Avenue, New York, NY 10016-5990; Order Department: 22 Law Drive, P.O. Box 2900, Fairfield, NJ 07007-2900 (www.asme.org)

Handbook of Chemistry and Physics, CRC Press, ISO, 74th ed., 1994-1995.

International Vocabulary of Basic and General Terms in Metrology (VIM), ISO, 2nd ed., 1993

Publisher: International Organization for Standardization (ISO), 1 ch. de la Voie-Creuse, Case postale 56, CH-1211, Genève 20, Switzerland/Suisse (www.iso.org)

9.2 References Cited In Text

The following sources were cited using numbered references throughout this document.

[1] L. V. King, "On the Convection of Heat From Small Cylinders in a Stream of Fluid: Determination of the Convection Constants of Small Platinum Wires With Application to Hot-Wire Anemometry," *Philosophical Transactions of the Royal Society*, A214 (1914): 373-432.

[2] ANSI/ASME MFC-1M-2003, "Glossary of Terms Used in the Measurement of Fluid Flow in Pipes."

[3] ANSI/ASME MFC-11M-2005, "Measurement of Fluid Flow by Means of Coriolis Mass Flowmeters."

[4] ANSI/ASME MFC-15M, "Insertion Metering."

[5] J. G. Olin, "A Thermal Mass Flow Monitor for Continuous Emissions Monitoring Systems (CEMS)," *Proceeding ISA/93 International Conference Exhibition and Training Program*, No. 93-404 (1993): 1635-1653.

[6] J. G. Olin, "Thermal Anemometry," Chapter 29.2 in J.G. Webster, *The Measurement, Instrumentation, and Sensors Handbook*, CRC Press (1999).

[7] N-T. Nguyen, "Thermal Mass Flow Sensors," Chapter 28.9 in J. G. Webster, *The Measurement, Instrumentation, and Sensors Handbook*, CRC Press (1999).

[8] H. H. Bruun, "Hot-Wire Anemometry: Principles and Signal Analysis," Oxford: *Oxford University Press* (1995).

[9] J. G. Olin, "Industrial Thermal Mass Flowmeters-Part 1: Principles of Operation," *Measurements and Control*, Issue 193, 83-90, February 1999.

[10] J. G. Olin, "Industrial Thermal Mass Flowmeters-Part 2: Applications," *Measurements and Control*, Issue 194, 1-6, April 1999.

[11] R. W. Miller, *Flow Measurement Engineering Handbook*, 3rd Edition, McGraw-Hill (1996).

[12] ANSI/ASME MFC-10M, "Installation Effects on Primary Devices."

[13] R. H. Dieck, *Measurement Uncertainty: Methods and Applications*, 2nd Ed., ISA (1997).

[14] ANSI/ASME MFC-17M, "Flow Measurement by Volumetric Method."

[15] ANSI/ASME MFC-9M, "Measurement of Liquid Flow in Conduits by Weighing Method."

[16] ISO 5168:2005(E) "Standard, Measurement of Fluid Flow," *Procedures for the Evaluation of Uncertainties*.

[17] ANSI/ASME MFC-2M, "Determination of Uncertainties."



INTENTIONALLY LEFT BLANK



MANDATORY APPENDIX I

FLOW CALIBRATION

I-1 INTRODUCTION

Because the critical dimensions of the flow sensor of thermal dispersion mass flowmeters are so small, manufacturing technology is currently incapable of maintaining sufficiently small tolerances to ensure reproducibility from flow sensor to flow sensor. Additionally, analog electronic components have variations and digital electronics have a fundamental digital resolution. For these reasons, every general purpose thermal dispersion mass flowmeter should be flow calibrated by the manufacturer, just like most other kinds of flowmeters. Exceptions may include thermal dispersion flow switches and low-accuracy flowmeters.

(a) The term “flow calibration” as used herein has the following definitions:

(1) the process of comparing the flowmeter’s indicated mass flow rate to a traceable flow calibration standard

(2) the process of adjusting the flowmeter’s output to bring it to a desired value, within a specified tolerance, for a particular value of the mass flow rate input

(b) Flow calibration falls into two categories:

(1) standard flow calibration — the details of which are specified by the manufacturer

(2) special flow calibration — the details of which are specified by the user

The majority of this Mandatory Appendix applies to gas flow calibration. Paragraph I-7 covers liquid flow calibration. The distinction between flow calibration of in-line versus insertion flowmeters is described in para. 4.7.1. The guidelines set forth in this Mandatory Appendix should be followed by all flow calibration entities: the manufacturer, the user, and third parties. The flow calibration laboratory should be accredited. It is preferred that the flow calibration laboratory have an ISO 9001 certification. It is advantageous that the flow calibration laboratory can demonstrate compliance with the latest revisions of ISO/IEC 17025 or ANSI Z540.

I-2 FLOW CALIBRATION CURVES

Figure 3.3-1 shows the flow calibration curves of typical thermal dispersion mass flowmeters. The curves are nonlinear and of a logarithmic nature. The nonlinearity is advantageous because it provides wide rangeability for a single flowmeter. It is disadvantageous because it requires several flow calibration points to properly define the calibration curve. It is recommended that the

flow calibrating entity use a procedure that fits a smooth curve through the data. References [8] and [13] provide insight into curve fitting.

I-3 FLOW CALIBRATION METHODS

I-3.1 Flow Calibration Facilities

Gas flow calibration facilities are of two types: open loop and closed loop. Figure I-1 shows a typical open-loop facility. Figure I-2 shows a typical closed-loop facility. Each figure lists the typical components of the facility. Two of their critical components: the flow conditioning section and the flow calibration standard, are given special attention in paras. I-3.2 through I-3.3.2.

Flow calibration facilities should be capable of the following:

(a) generating a stable, steady-state, reproducible gas mass flow rate.

(b) accommodating with required accuracy the entire mass flow range specified. If extrapolation has been used to extend the range, this information should be made available to the user upon request.


(c) reproducing the gas composition, temperature, and pressure to be encountered in the actual application. Closed-loop facilities, such as that shown in Fig. I-2, are designed to accomplish this objective. Alternately, a surrogate, or reference gas may be used at reference temperature and pressure conditions.

It should be noted by the flow-calibrating entity that the simplest flow calibration facility (an open-loop air flow facility with a fan as the flow generator) actually is a closed-loop facility with the loop closing within the laboratory. For air velocities less than about 5 m/s, such ambient pressure flow calibration facilities can experience shifts due to the opening and closing of doors to the room and other causes of pressure and temperature changes in the room. Operators of such facilities should minimize and account for the effect of such variations on the accuracy of flowmeters.

I-3.2 Flow-Conditioning Section

The flow-conditioning section is an essential, but often overlooked, component of the flow calibration facilities shown in Figs. I-1 and I-2. Its purpose is to condition the flow prior to the flow entering the flowmeter under test. The flow-conditioning section should have the following attributes.

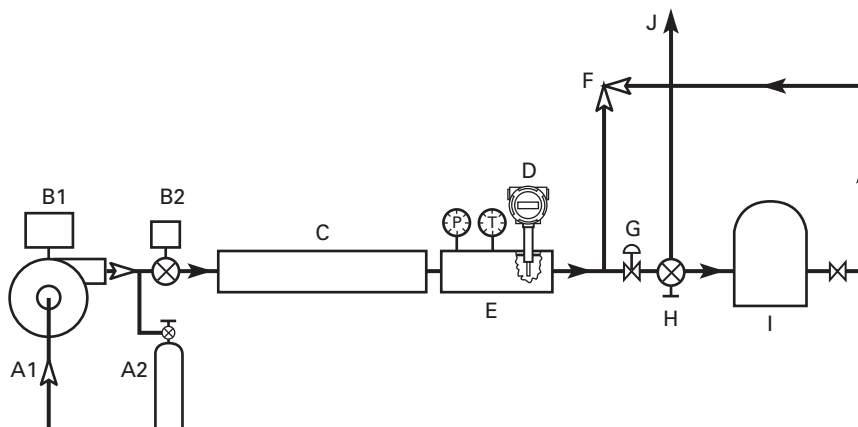

Fig. I-1 Typical Open Loop Gas Calibration Facility**LEGENDS:**

- A1 = Flow source (air blower or pump).
- A2 = Alternative flow source (pressurized gas tank).
- B1 = Flow controller (variable speed motor drive).
- B2 = Alternative flow controller (flow control valve).
- C = Flow conditioning section (see para I-3.2).
- D = Flowmeter under test (insertion meter shown).
- E = Test section (part of flow conditioning section; for insertion flowmeters only; see para I-3.2).
- F = Pressure relief valve (for pressurized facilities only).
- G = Pressure regulator (for pressurized facilities only).
- H = Diverter valve (for batching calibration standards only).
- I = Flow calibration standard (either batching or in-line).
- J = Vent (leads to outside environment or to scrubber or other gas purifying device).

(a) For in-line flowmeters, the flow-conditioning section should be straight pipe with lengths upstream and downstream of the flowmeter under test that meet the minimum specification requirements specified by the manufacturer. A flow straightening and swirling flow eliminating device may be required upstream of the upstream pipe.

(b) For insertion flowmeters installed in pipes with fully developed velocity profiles, the flow-conditioning section should be a length of straight pipe upstream of the flowmeter under test that is sufficiently long to create a fully developed velocity distribution.

(c) For insertion flowmeters in large flow conduits and in general applications, it is recommended that the flow-conditioning section is capable of generating a flat, quiet, nonswirling velocity profile. In this case, the preferred flow-conditioning section has the following components:

(1) a flow-quieting section, such as a plenum with a flow straightener and screens or other means that reduce flow nonuniformities.

(2) a nozzle to further flatten the velocity profile.

(3) a test section consisting of either a straight walled section or a free jet into which the flow sensor of the insertion flowmeter under test is inserted. The test section should have a velocity profile that is uniform

in the central two-thirds portion within approximately 0.5% to 1%; a turbulence intensity less than about 0.5%; and a cross-sectional area large enough so that the flow blockage ratio is less than approximately 5%.


I-3.3 Flow Calibration Standard

It is recommended that the flow calibration standard component of the flow calibration facility have an accuracy at least 3 times better (i.e., an uncertainty of one-third, or less) than that specified for the flowmeter under test. Flow calibration of the flow calibration standard should be traceable to a recognized national or international measurement standard, and its most recent traceable accuracy should be documented. This information should be made available by the manufacturer, upon the user's request.

Flow calibration standards that measure volumetric flow rate or displaced volume should have temperature and pressure transducers located close to the entrance of the flow calibration standard, but with no flow obstruction. These measurements are used to compute the mass density ρ of the gas (i.e., in units of kg/m^3), as in para. 4.7.10. The mass density, ρ , is then used to compute the mass flow rate q_m , as shown in subsequent sections.



Fig. I-2 Typical Closed Loop Gas Calibration Facility

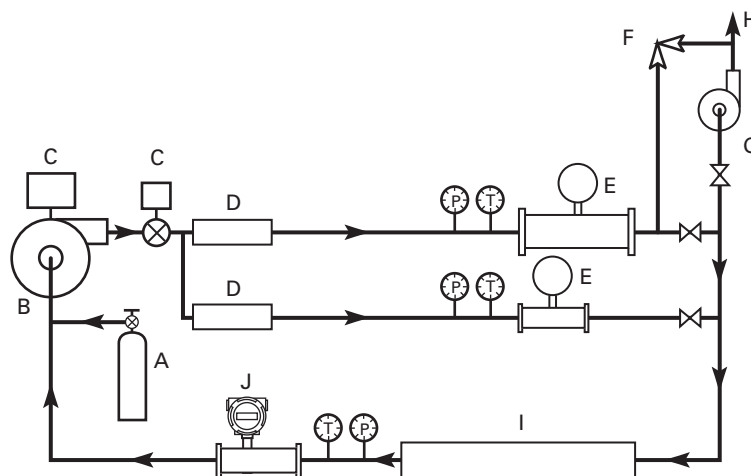

LEGENDS:

- A = Gas source (for pressurized facilities – compressed air or pressurized gas tank; for air wind tunnels – no “gas source” is used).
 B = Flow source (for pressurized facilities – high pressure axial or centrifugal pump; for air wind tunnel – fan or blower).
 C = Flow controller (variable speed motor drive; or flow control valve).
 D = Flow conditioning section [for flow calibration standard(s)].
 E = Flow calibration standard(s) (in-line only; multiple sized standards may be used to extend rangeability; see para I-3.3.1).
 F = Pressure relief valve.
 G = Vacuum pump (evacuates gas in system prior to gas filling).
 H = Vent (leads to outside environment or to scrubber or other gas purifying device).
 I = Flow conditioning section (see para I-3.2).
 J = Flowmeter under test (for insertion or in-line flowmeters; in-line flowmeter shown).

Flow calibration standards are of two types

- (a) in-line flow calibration standards: used in both open-loop and closed-loop flow calibration facilities
- (b) batching flow calibration standards: used in open-loop flow calibration facilities

I-3.3.1 In-Line Flow Calibration Standards. Typical in-line flow calibration standards that measure the volumetric flow rate, q_v (e.g., in units of m^3/s), include rotating and reciprocating positive displacement flowmeters; turbine flowmeters; multipath ultrasonic flowmeters; venturi flowmeters; flow nozzles; and sonic nozzles. The desired mass flow rate is computed as $q_m = \rho q_v$ (kg/s).

Typical in-line flow calibration standards that directly measure the mass flow rate q_m include

- (a) Coriolis mass flowmeters
- (b) specially calibrated thermal dispersion mass flowmeters
- (c) specially calibrated capillary tube thermal mass flowmeters

Flow calibration of a thermal dispersion mass flowmeter with another specially calibrated thermal dispersion mass flowmeter should be performed with caution because influence parameters may affect each flowmeter in a similar manner (bias) that may not be indicated in the flow calibration result.

I-3.3.2 Batching Flow Calibration Standards. Typical batching flow calibration standards measure the volume

of the flow calibration gas passing through the flowmeter under test [14]. Typical flow calibration standards of this kind are positive displacement flow calibrators, or volumetric provers, such as bell provers and piston provers. In these flow calibrators, the displaced volume Vol (e.g., in units of m^3) and the time of transit Δt (e.g., in units of seconds) of the bell or piston are measured and used to compute the desired mass flow rate as $q_m = \rho Vol / \Delta t$ (kg/s).

Vol and Δt should be measured only during the steady-state rise of the bell or piston (i.e., after their initial acceleration and before their final deceleration). The transit time Δt should be sufficiently long so that both the resolution of the Δt measurement and small flow rate variations have negligible effect. Because the size of batching flow calibration standards is limited, their use should be relegated to gas mass flow rates in the lower ranges. In-line standards should be used for higher ranges.

I-4 FLOW CALIBRATION PROCEDURES

All flow calibrating entities should adopt the following procedures:

- (a) The flowmeter under test is installed in accordance with the manufacturer's recommendations (see para. 6.1).



(b) The flow calibration is preceded by an appropriate warm-up period for each flow rate calibration data point.

(c) All transmitter configuration data is recorded prior to the start of the test.

(d) The test flow rates are selected to ensure that the flowmeter's performance meets its specification over the operating flow range.

(e) The calibration of the flow calibration standard is current and traceable.

(f) The uncertainty of the flow calibration standard is recommended to be one-third, or better, than the uncertainty of the specification for the flowmeter under test.

(g) The flow rate is maintained constant while a data point is being taken. This is especially important if a batching flow calibration standard is used.

(h) The zero value is measured and only when there is absolutely no flow in the facility and, if possible, at process pressure and temperature.

(i) Variations in gas temperature and pressure are minimized during the flow calibration process. The gas temperature should be held within approximately $\pm 3^{\circ}\text{C}$ ($\pm 5.4^{\circ}\text{F}$) during flow calibration. The gas pressure should be held within approximately ± 0.2 bar (± 3 psi).

I-5 CALIBRATION CERTIFICATE

For every flowmeter the flow calibrating entity should provide the user a certificate that includes the following data:

- unique certificate number, repeated on each page along with the page number and the total number of pages
- calibration date
- certificate's date of issue
- identity of the party commissioning the calibration
- name and location of the flow calibration laboratory

- test gas data and the test temperature, pressure, etc.
- calibration laboratory's basic methodology of flow calibration (see para. I-3)
- unique identification of the flowmeter under test
- traceability of the flow calibration facility
- reference identifying the flow calibration laboratory's documentation and how it can be reviewed
- uncertainty statement for the flow calibration laboratory
- relevant ambient conditions
- name of the calibration operator
- configuration data within the transmitter when the calibration was performed
- table showing all mass flow rate data including the temperature, pressure, and other measurements taken concurrently

I-6 FREQUENCY OF RECALIBRATION

Thermal dispersion mass flowmeters generally require infrequent flow recalibration. The manufacturer should inform the user of the typical recalibration frequency for their application. The frequency of recalibration is governed by the criticality of the measurement, the nature of the operating conditions, the level of confidence required by the user, and the stability of the flow sensor. For fiscal and custody transfer applications, a higher recalibration frequency is recommended. If the installation conditions change, such as the result of pipe work modifications in the vicinity of the flowmeter, recalibration may be required.

I-7 LIQUID FLOW CALIBRATION

Liquid flow calibration systems fall into three categories: gravimetric, volumetric, or in-line flow calibration. Many of the gas flow calibration procedures in the preceding sections are applicable to liquid flow calibration. Liquid flow calibration is thoroughly described in the open literature (e.g., references [3, 14, 15]).

NONMANDATORY APPENDIX A

IN-LINE FLOWMETER SIZING AND PERMANENT PRESSURE LOSS

A-1 IN-LINE FLOWMETER SIZING

Table A-1 shows the mass flow rates for in-line thermal dispersion mass flowmeters in sizes ranging from 0.25 in. to 8 in. (DN 6 to DN 200 mm) and with a built-in flow conditioner. Manufacturers should be consulted for applications requiring higher ranges.

the permanent pressure loss for typical in-line flowmeters in sizes ranging from 0.25 in. to 8 in. (DN 6 to DN 200 mm) and with a built-in flow conditioner. Manufacturers should be consulted for applications requiring lower permanent pressure losses.

A-2 PERMANENT PRESSURE LOSS

Paragraph 5.4 discusses the permanent pressure loss of in-line and insertion flowmeters. Figure A-1 shows


Table A-1 Sizes and Mass Flow Rates for Typical In-Line Flowmeters

Pipe Size (in.)	Air and Nitrogen Mass Flow Rate Ranges			
	Minimum Range		Maximum Range	
	Scfm [Note (1)]	normal m ³ /h [Note (2)]	Scfm [Note (1)]	normal m ³ /h [Note (2)]
0.25	0–0.5	0–0.7	0–9	0–14
0.5	0–2	0–3.0	0–40	0–60
0.75	0–4	0–5.9	0–75	0–120
1.0	0–6	0–8.9	0–120	0–180
1.5	0–15	0–22	0–280	0–440
2.0	0–23	0–33	0–470	0–680
3.0	0–50	0–74	0–1000	0–1500
4.0	0–90	0–130	0–1800	0–2700
6.0	0–200	0–300	0–4000	0–5900
8.0	0–350	0–520	0–7000	0–10000

NOTES:

- (1) At base conditions of 21.1°C temperature and 1 atm pressure.
- (2) At base conditions of 0°C temperature and 1 atm pressure.

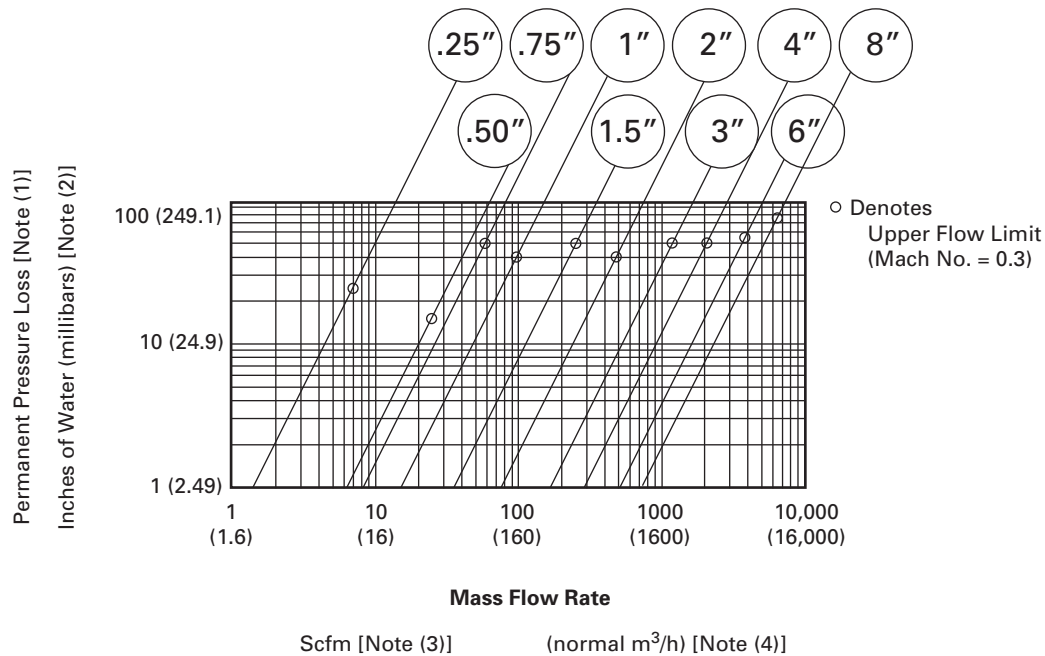

Fig. A-1 An Example of Permanent Pressure Loss for In-Line Flowmeters With a Built-In Flow Conditioner

GENERAL NOTE: Built-in flow conditioner consists of two separate perforated plates in series.

NOTES:

- (1) For air and nitrogen at 20°C and 1 atm pressure.
- (2) 1 in. of water at 60°F = 0.0361 psi.
- (3) At base conditions of 21.1°C and 1 atm pressure.
- (4) At base conditions of 0°C and 1 atm.

NONMANDATORY APPENDIX B ACCURACY AND UNCERTAINTY

B-1 INTRODUCTION

Paragraph 5.6.1 of the main text provides a general discussion of the accuracy of mass flow rate measurement. This Nonmandatory Appendix presents an example calculation of overall accuracy and a simplified discussion of uncertainty.

B-2 EXAMPLE ACCURACY CALCULATION

This section gives a typical numerical calculation of the overall accuracy, A_t , including the use of the temperature influence coefficient, C_T , and the pressure influence coefficient, C_P . It is based on eq. (5-3) in the main text.

If both T and P fall outside their reference condition range, the overall accuracy (in units of percent of reading) based on eq. (5-3) is as follows:

$$A_t = \pm[A_r + A_{fs} q_{m,fs} / q_m + C_T \text{Abs}(T_f - T_L) + C_P \text{Abs}(P - P_L)] \quad (\text{B-1})$$

where

$\text{Abs}()$ = absolute value of the difference in parentheses

P_L = the upper or lower limit of the pressure reference condition range

T_L = the upper or lower limit of the temperature reference condition range

EXAMPLE: Assume that a thermal dispersion mass flowmeter is flow calibrated at 20°C and 5 bar, but the process temperature for T_f is 40°C and the process pressure P is 7 bar. Further assumptions are:

A_r = 1.0% of reading over 10% to 100% of full scale range

A_{fs} = 0.5% of full scale over 10% to 100% of full scale range

Addition assumptions are: Actual mass flow rate q_m is 80% of the full scale value $q_{m,fs}$. Reference temperature range is $\pm 10^\circ\text{C}$ of the flow calibration temperature. Reference pressure range is ± 1 bar of the flow calibration pressure. Temperature influence coefficient, C_T , is 0.04%

of reading per degree centigrade for actual temperatures in the range of $\pm(10^\circ\text{C}$ to $25^\circ\text{C})$ of the flow calibration temperature. Pressure influence coefficient, C_P , is 0.3% of reading per bar for actual pressure in the range of $\pm(1$ bar to 16 bar) of the flow calibration pressure.

The overall accuracy is calculated as follows:

$$A_t = \pm[1.0 + 0.5 / 0.8 + 0.04 \times (40 - 30) + 0.3 \times (7 - 6)]$$

$$A_t = \pm 2.325\% \text{ of reading}$$

B-3 DISCUSSION OF UNCERTAINTY

The uncertainty of flowmeters is covered in detail in the open literature [3, 13, 16, 17]. Following is a general expression of measurement uncertainty of thermal dispersion mass flowmeters.

In general, the mass flow rate, q_m , is a function of n input variables x_i , as follows:

$$q_m = f(x_1, x_2, \dots, x_n) \quad (\text{B-2})$$

The uncertainty in q_m is expressed as $u(q_m)$. If the errors are random and are not systematic (i.e., there is no bias), then the uncertainty in the mass flow rate of thermal dispersion mass flowmeters is expressed as follows:

$$u(q_m) = t[\sum(S_i^2 u(x_i)^2)]^{1/2} \text{ for } i=1,2,\dots,n \quad (\text{B-3})$$

where

$S_i = \delta q_m / \delta x_i$ = the sensitivity coefficient of q_m to input variable x_i

$t = t_{68}$ or t_{95} = the factor from the student's t distribution required to yield an uncertainty in q_m with a confidence level of 68.3% or 95.5%, respectively. For more than 10 deg of freedom, the following values of t are used: $t_{68} = 1$ and $t_{95} = 2$. t_{68} yields the one-sigma uncertainty value, and t_{95} yields the two-sigma uncertainty value.

$u(x_i)$ = the uncertainty of input variable x_i



INTENTIONALLY LEFT BLANK



ASME Services

ASME is committed to developing and delivering technical information. At ASME's Information Central, we make every effort to answer your questions and expedite your orders. Our representatives are ready to assist you in the following areas:

ASME Press
Codes & Standards
Credit Card Orders
IMEchE Publications
Meetings & Conferences
Member Dues Status

Member Services & Benefits
Other ASME Programs
Payment Inquiries
Professional Development
Short Courses
Publications

Public Information
Self-Study Courses
Shipping Information
Subscriptions/Journals/Magazines
Symposia Volumes
Technical Papers

How can you reach us? It's easier than ever!

There are four options for making inquiries* or placing orders. Simply mail, phone, fax, or E-mail us and an Information Central representative will handle your request.

Mail
ASME
22 Law Drive, Box 2900
Fairfield, New Jersey
07007-2900

Call Toll Free
US & Canada: 800-THE-ASME
(800-843-2763)
Mexico: 95-800-THE-ASME
(95-800-843-2763)
Universal: 973-882-1167

Fax—24 hours
973-882-1717
973-882-5155

E-Mail—24 hours
Infocentral@asme.org

* Information Central staff are not permitted to answer inquiries about the technical content of this code or standard. Information as to whether or not technical inquiries are issued to this code or standard is shown on the copyright page. All technical inquiries must be submitted in writing to the staff secretary. Additional procedures for inquiries may be listed within.



INTENTIONALLY LEFT BLANK



INTENTIONALLY LEFT BLANK



ASME MFC-21.2–2010

ISBN 978-0-7918-3308-7



K15610

Copyright © 2011 by the American Society of Mechanical Engineers.
No reproduction may be made of this material without written consent of ASME.

