



Standard Practice for Using a Guarded-Hot-Plate Apparatus or Thin-Heater Apparatus in the Single-Sided Mode¹

This standard is issued under the fixed designation C1044; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This practice covers the determination of the steady-state heat flow through the meter section of a specimen when a guarded-hot-plate apparatus or thin-heater apparatus is used in the single-sided mode of operation.

1.2 This practice provides a supplemental procedure for use in conjunction with either Test Method C177 or C1114 for testing a single specimen. This practice is limited to only the single-sided mode of operation, and, in all other particulars, the requirements of either Test Method C177 or C1114 apply.

NOTE 1—Test Methods C177 and C1114 describe the use of the guarded-hot-plate and thin-heater apparatus, respectively, for determining steady-state heat flux and thermal transmission properties of flat-slab specimens. In principle, these methods cover both the double- and single-sided mode of operation, and at present, do not distinguish between the accuracies for the two modes of operation. When appropriate, thermal transmission properties shall be calculated in accordance with Practice C1045.

1.3 This practice requires that the cold plates of the apparatus have independent temperature controls. For the single-sided mode of operation, a (single) specimen is placed between the hot plate and the cold plate. Auxiliary thermal insulation, if needed, is placed between the hot plate and the auxiliary cold plate. The auxiliary cold plate and the hot plate are maintained at the same temperature. The heat flow from the meter plate is assumed to flow only through the specimen, so that the thermal transmission properties correspond only to the specimen.

NOTE 2—The double-sided mode of operation requires similar specimens placed on either side of the hot plate. The cold plates that contact the outer surfaces of these specimens are maintained at the same temperature. The electric power supplied to the meter plate is assumed to result in equal heat flow through the meter section of each specimen, so that the thermal transmission properties correspond to an average for the two specimens.

1.4 This practice does not preclude the use of a guarded-hot-plate apparatus in which the auxiliary cold plate is either larger or smaller in lateral dimensions than either the test specimen or the cold plate.

¹ This practice is under the jurisdiction of ASTM Committee C16 on Thermal Insulation and is the direct responsibility of Subcommittee C16.30 on Thermal Measurement.

Current edition approved Sept. 1, 2016. Published September 2016. Originally approved in 1985. Last previous edition approved in 2012 as C1044 – 12. DOI: 10.1520/C1044-16.

NOTE 3—Most guarded-hot-plate apparatus are designed for the double-sided mode of operation (1).² Consequently, the cold plate and the auxiliary cold plate are the same size and the specimen and the auxiliary insulation will have the same lateral dimensions, although the thicknesses need not be the same. Some guarded-hot-plate apparatus, however, are designed specifically for testing only a single specimen that is either larger or smaller in lateral dimensions than the auxiliary insulation or the auxiliary cold plate.

1.5 This practice is suitable for use for both low- and high-temperature conditions.

1.6 This practice shall not be used when operating an apparatus in a double-sided mode of operation with a known and unknown specimen, that is, with the two cold plates at similar temperatures so that the temperature differences across the known and unknown specimens are similar.

1.7 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*³

C168 Terminology Relating to Thermal Insulation³

C177 Test Method for Steady-State Heat Flux Measurements and Thermal Transmission Properties by Means of the Guarded-Hot-Plate Apparatus³

C518 Test Method for Steady-State Thermal Transmission Properties by Means of the Heat Flow Meter Apparatus³

C1045 Practice for Calculating Thermal Transmission Properties Under Steady-State Conditions³

C1114 Test Method for Steady-State Thermal Transmission Properties by Means of the Thin-Heater Apparatus

3. Terminology

3.1 *Definitions*—For definitions of terms used in this practice, refer to Terminology C168. For definitions of terms

² The boldface numbers in parentheses refer to the list of references at the end of this standard.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

relating to the guarded-hot-plate apparatus or thin-heater apparatus refer to Test Methods C177 or C1114, respectively.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *auxiliary cold plate, n*—the plate that provides an isothermal boundary at the outside surface of the auxiliary insulation.

3.2.2 *auxiliary insulation, n*—thermal insulation used in place of a second test specimen, when the single-sided mode of operation is used (syn. dummy specimen).

3.2.3 *cold plate, n*—the plate that provides an isothermal boundary at the cold surface of the specimen.

3.2.4 *double-sided mode, n*—operation of the apparatus, such that the heat input to the meter plate flows equally through two specimens, each specimen placed on either side of the hot plate (see also **single-sided mode**).

3.2.5 *gap, n*—separation between the meter plate and guard plate, usually filled with a gas or thermal insulation.

3.2.6 *guard plate, n*—the outer (rectangular or circular) ring of the guarded hot plate, that encompasses the meter plate and promotes one-dimensional heat flow normal to the meter plate.

3.2.7 *guarded hot plate, n*—an assembly, consisting of a meter plate and a co-planar, concentric guard plate, that provides the heat input to the specimen(s).

3.2.8 *meter plate, n*—the inner (rectangular or circular) plate of the guarded hot plate, that provides the heat input to the meter section of the specimen(s).

3.2.9 *meter section, n*—the portion of the specimen (or auxiliary insulation) through which the heat input to the meter plate flows under ideal guarding conditions.

3.2.10 *single-sided mode, n*—operation of the apparatus such that essentially all of the heat input to the meter plate flows through a specimen placed on one side of the hot plate (see also **double-sided mode**).

3.2.11 *thin heater, n*—an assembly, consisting of an unpartitioned thin-screen heater or thin-foil, that provides the heat input to the specimen(s).

3.3 *Symbols*—The symbols used in this practice have the following significance. The prime (') denotes quantities associated with the auxiliary insulation used to control heat from the other side of the hot plate.

3.3.1 A —meter area of hot plate, m^2 .

3.3.2 C' —thermal conductance of auxiliary insulation, $W/(m^2 \cdot K)$.

3.3.3 Q —heat flow through meter section of specimen, W .

3.3.4 Q' —heat flow through meter section of auxiliary insulation, W .

3.3.5 Q_m —power input to meter plate, W .

3.3.6 T_c —surface temperature of cold plate, K .

3.3.7 T'_c —surface temperature of auxiliary cold plate, K .

3.3.8 T_h —surface temperature of hot plate in contact with specimen, K .

3.3.9 T'_h —surface temperature of hot plate in contact with auxiliary insulation, K .

4. Significance and Use

4.1 This practice provides a procedure for operating the apparatus so that the heat flow, Q' , through the meter section of the auxiliary insulation is small; determining Q' ; and, calculating the heat flow, Q , through the meter section of the specimen.

4.2 This practice requires that the apparatus have independent temperature controls in order to operate the cold plate and auxiliary cold plate at different temperatures. In the single-sides mode, the apparatus is operated with the temperature of the auxiliary cold plate maintained at the same temperature of the hot plate face adjacent to the auxiliary insulation.

NOTE 4—In principle, if the temperature difference across the auxiliary insulation is zero and there are no edge heat losses or gains, all of the power input to the meter plate will flow through the specimen. In practice, a small correction is made for heat flow, Q' , through the auxiliary insulation.

4.3 The thermal conductance, C' , of the auxiliary insulation shall be determined from one or more separate tests using either Test Method C177, C1114, or as indicated in 5.4. Values of C' shall be checked periodically, particularly when the temperature drop across the auxiliary insulation less than 1 % of the temperature drop across the test specimen.

4.4 This practice is used when it is desirable to determine the thermal properties of a single specimen. For example, the thermal properties of a single specimen are used to calibrate a heat-flow-meter apparatus for Test Method C518.

5. Procedure for Single-Sided Mode of Operation

5.1 Refer to Fig. 1 for a schematic diagram of the single-sided mode of operation of the guarded-hot-plate apparatus.

NOTE 5—The schematic diagram for a thin-heater apparatus (not shown) is similar, except the hot plate is much thinner and is not partitioned by a gap.

5.2 Follow the procedure of either Test Method C177 or C1114 with the following modifications.

5.3 Select a rigid or semi-rigid material for the auxiliary insulation having a low thermal conductance so that heat gains or losses from the face of the meter plate in contact with the auxiliary insulation will be small. The thickness and lateral conductance of the auxiliary insulation shall be small to avoid significant effects on the heat transfer through the meter section of the auxiliary insulation due to heat transfer at the edge of the auxiliary insulation.

NOTE 6—The influence of edge effects for a particular apparatus and test configuration is determined experimentally as described in Test Method C177 or by computation using one of the procedures referenced in Test Method C177 or described by Peavy and Rennex (2).

5.4 Determine C' of the auxiliary insulation over the temperature range of interest using one of the following procedures: (1) Test Method C177 or C1114 in a separate test setup for a matched pair of similar specimens; or (2) in-situ as described in Annex A1.

5.4.1 In the first instance, using either Test Method C177 or C1114, a matched pair of similar specimens is required so that either single specimen subsequently is suitable for use as the auxiliary insulation.

Guarded - Hot - Plate Apparatus

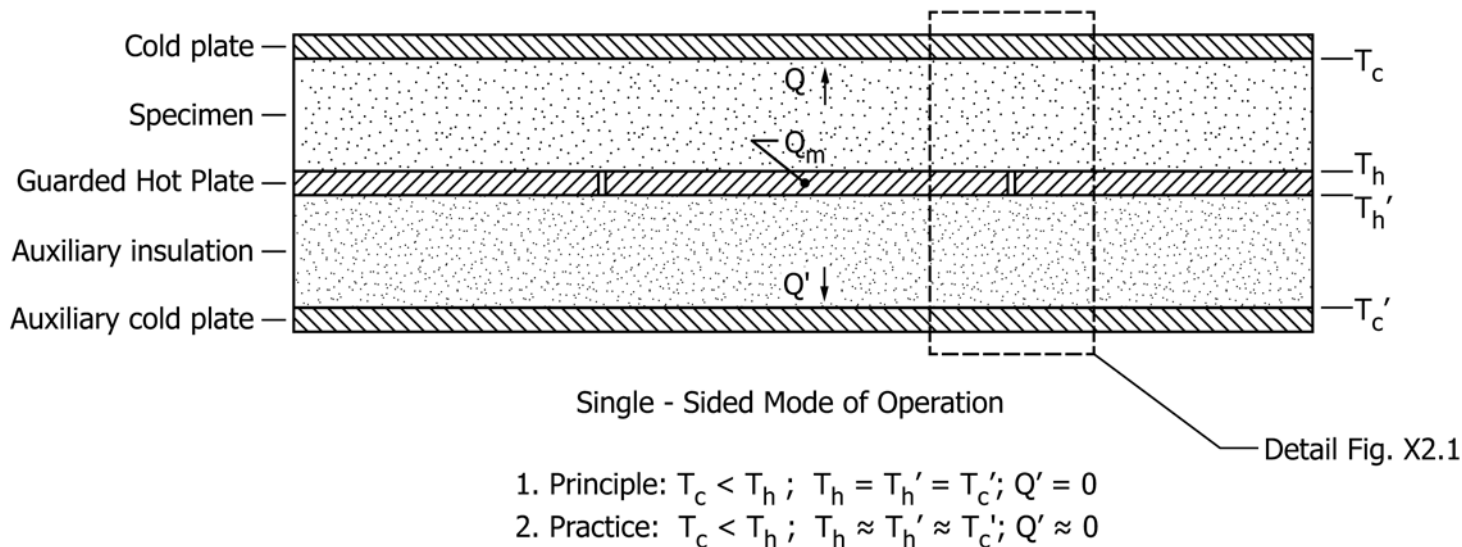


FIG. 1 Diagram Illustrating Single-Sided Mode of Operation of the Guarded-Hot-Plate Apparatus

5.4.2 In the second instance using in-situ as described in **Annex A1**, successive tests are required, one with a small temperature difference across the test specimen and one with a small temperature difference across the auxiliary insulation.

NOTE 7—In 5.4 the user is not required to determine values for C' for every test that will be conducted. Rather, determine C' as a function of temperature over the temperature range of interest so that a corresponding regression curve is developed for subsequent testing.

5.5 When using a compressible material as the auxiliary insulation, determine C' either at the same thickness as that used in the single-sided mode of operation or compressed to (at least) two slightly different thicknesses, thus allowing interpolation for the thickness actually used in the single-sided mode of operation.

5.5.1 For an apparatus without a separate provision for determining the individual thicknesses of the two specimens on opposite sides of the hot plate, place three or more low-conductance rigid spacers near the outer periphery of the guard plate between the hot plate and the surface of the auxiliary cold plate.

5.5.2 Compute the effective thickness of the test specimen by subtracting the thickness of the rigid spacers (corrected for thermal expansion, if necessary) from the thickness that is determined for the test specimen plus the auxiliary insulation. In this case, the separate tests of thermal conductance according to 5.4.2 shall be conducted with rigid spacers.

5.6 Maintain the cold plate at the required temperature T_c . Provide power input to the hot plate to attain the required temperature T_h on the hot side of the test specimen.

5.7 Maintain the temperature T_c' as closely as practical to the temperature T_h .

5.8 Establish thermal steady-state conditions in accordance with either Test Method **C177** or **C1114**.

5.9 Acquire the required test data and determine A , Q_m , T_h , T_h' , and T_c' in accordance with either Test Method **C177** or **C1114**.

6. Calculation

6.1 Calculate the heat flow through the auxiliary insulation as follows:

$$Q' = C' A (T_h' - T_c') \quad (1)$$

where:

C' is the thermal conductance of the auxiliary insulation at a temperature corresponding to $(T_h' + T_c')/2$, as obtained according to 5.4.

6.2 Calculate the heat flow through the specimen as follows:

$$Q = Q_m - Q' \quad (2)$$

6.3 Use the value of Q , thus obtained to calculate steady-state thermal transmission properties, in accordance with either Test Method **C177** or **C1114**. When appropriate, consult Practice **C1045** to calculate steady-state thermal transmission properties. For reference, calculation equations are provided in **Appendix X1**.

7. Sources of Experimental Error

7.1 Errors in the determination of Q , are introduced from several sources, including measurement of the power input Q_m to the meter plate; estimation of the heat flow, Q' , through the auxiliary insulation and, for guarded hot plates, estimation of the heat flow across the gap between the meter plate and guard plate, that is, gap error.

7.2 Refer to either Test Method **C177** or **C1114** for discussion on the uncertainty in the measurement of the metered-area power (Q_m).

7.3 Estimate the uncertainty ($\Delta Q'$) in Q' by a propagation of error using the terms in Eq 1. Refer to Ku (3) for using error propagation formulas.

NOTE 8—When the terms Q_m and Q' in Eq 2 are different by at least two orders of magnitude, a large uncertainty in Q' results in a small uncertainty in Q . For example, suppose that the ratio Q_m/Q' is 100 and suppose that the ratio $\Delta Q'/Q'$ is 0.1. The percentage uncertainty in Q due to $\Delta Q'$, then, would be 0.1 %.

7.4 Refer to Appendix X2 for a discussion of the gap error.

7.5 Refer to Appendix X3 for a discussion on Precision and Bias and Measurement Uncertainty.

8. Report

8.1 Report all measurements in accordance with either Test Method C177 or C1114. Perform all calculations in accordance

with Practice C1045. The report shall note that the apparatus was operated in a single-sided mode in accordance with Practice C1044 and, in addition, the report shall include, where applicable, values for quantities associated with the auxiliary insulation, including Q' , T'_c and T'_h . The report shall include a description of the apparatus and the procedure for determining C' in 5.4.

9. Keywords

9.1 guarded-hot-plate apparatus; heat flow; single-sided; steady state; thermal insulation; thin-heater apparatus

ANNEX

(Mandatory Information)

A1. IN-SITU DETERMINATION OF THERMAL CONDUCTANCE OF AUXILIARY INSULATION

A1.1 This annex describes an iterative procedure for determining the thermal conductance of the auxiliary insulation from test data acquired with the hot-plate apparatus operated in the single-sided mode.

A1.2 Procedure:

A1.2.1 Install the auxiliary insulation and specimen in the apparatus. Conduct the following sequence of tests over the temperature range of interest.

A1.2.2 Following the procedure of Sections 5 and 6, calculate the thermal conductance, C , of the test specimen at a mean temperature corresponding to $(T_h + T_c)/2$. Determine C for at least three values of mean temperature over the temperature range of interest selected in A1.2.1.

A1.2.2.1 For the first iteration, the user shall estimate a value for C' based on experience, handbook data, etc.

A1.2.3 Using the same temperature range selected in A1.2.1, establish a small temperature difference, $T_h - T_c$, for example, $<2\text{ K}$ across the specimen and a significant temperature difference, $T'_h - T'_c$, for example, 20 K to 30 K across the auxiliary insulation.

A1.2.4 Calculate the heat flow through the specimen as follows:

$$Q = CA(T_h - T_c) \quad (\text{A1.1})$$

where:

C is the thermal conductance of the test specimen at a temperature corresponding to $(T_h + T_c)/2$, as determined in A1.2.2. Interpolation for the value of C will potentially be required.

A1.2.5 Calculate the heat flow through the auxiliary insulation as follows:

$$Q' = Q_m - Q \quad (\text{A1.2})$$

A1.2.6 Using the value of Q' , thus obtained, calculate the thermal conductance of the auxiliary insulation, C' , corresponding to a mean temperature of $(T'_h + T'_c)/2$. Determine C' for at least three values of mean temperature.

A1.2.7 Repeat A1.2.2 through A1.2.6 until successive values of C' vary by no more than 1 %.

APPENDIXES

(Nonmandatory Information)

X1. THERMAL TRANSMISSION EQUATIONS

X1.1 For reference, equations for calculating thermal transmission properties are provided in [X1.2](#).

X1.2 *Symbols*—The following symbols refer to equations in [Appendix X1](#).

A = meter area of hot plate, m^2 .
 Q = heat flow through meter section of test specimen, W .
 C = thermal conductance of specimen, $W/(m^2 \cdot K)$.
 R = thermal resistance of specimen, $(m^2 \cdot K)/W$.
 λ = thermal conductivity of specimen, $W/(m \cdot K)$

r = thermal resistivity of specimen, $(m \cdot K)/W$
 L = specimen thickness, m .
 T_c = surface temperature of cold plate, K .
 T_h = surface temperature of hot plate in contact with test specimen, K .

$$C = Q/A(T_h - T_c) \quad (X1.1)$$

$$R = (A(T_h - T_c))/Q \quad (X1.2)$$

$$\lambda = (LQ)/(A(T_h - T_c)) \quad (X1.3)$$

$$r = (A(T_h - T_c))/(LQ) \quad (X1.4)$$

X2. DISCUSSION OF ERROR DUE TO GAP HEAT FLOW IN A GUARDED-HOT-PLATE APPARATUS

X2.1 An error occurs due to lateral heat flows across the gap when a guarded-hot-plate apparatus designed for operation in a double-sided mode is used in a single-sided mode. This appendix discusses the sources for this error and procedures to estimate its magnitude.

NOTE X2.1—Error resulting from heat flow across the gap due to a temperature imbalance between the meter plate and guard plate is also discussed in Test Method [C177](#).

X2.2 Most guarded hot plates are constructed with a distributed heat source and surface plates of metal on either side of the heater core. When operated in a double-sided mode of operation, the symmetrical construction will result in the surfaces on either side of the meter plate attaining nearly the same temperature; however, when operated in a single-sided mode, the temperature of the side of the meter plate that contacts the auxiliary insulation is significantly hotter than the side that contacts the test specimen.

X2.3 For illustration, [Fig. X2.1](#) shows the heat flows in the region of the gap of a guarded-hot-plate apparatus under conditions when temperature differences are present. Path A represents heat flow through the region of the test specimen that is in close proximity to the gap. Similarly, Path E represents heat flow through the auxiliary specimen. Paths B, C, and D correspond to heat flows across portions of the gap on the test specimen side, in the center, and on the auxiliary specimen side, respectively.

X2.4 The critical requirement for eliminating heat flow across the gap is the proper design of the guarded hot plate and installation of the temperature sensors, such that the net heat flow between the meter and guard plates, integrated over all paths, be zero when the measured temperature difference is, in fact, zero.

X2.5 Hypothetical Example:

X2.5.1 [Fig. X2.2](#) shows the cross section, near the gap, of a (hypothetical) guarded hot plate designed for double-sided

mode of operation. The meter and guard plates are identical in construction having a symmetrical heater core with (wire or ribbon) heaters electrically insulated from metal surface plates. The two heaters are part of a single winding and cannot be operated separately. The thermopile used to control the temperature of the guard plate, relative to the temperature of the meter plate, has its junctions located in the surface plates ([Fig. X2.2a](#)).

NOTE X2.2—Actual designs of guarded hot plates need not be the same as the hypothetical design shown in [Fig. X2.2](#). This simple design was selected to illustrate the differences in temperature profiles that can arise when equipment designed for operation in a double-sided mode is used in a single-sided mode.

X2.5.2 *Double-Sided Mode*—The first temperature profile shown in [Fig. X2.2b](#) illustrates the variation in spatially averaged temperature through the guarded hot plate when it is operated in the double-sided mode with identical heat fluxes on each side. The surface plates of metal have a high thermal conductivity and are presumed isothermal. The temperature gradient across the electrical insulating layer between each heater and the corresponding surface plate is due to the heat flow from that heater into the test specimen (not shown) in contact with the surface plate. The region between the heaters, on average, is isothermal since the net heat flow in or out of the region is zero. The temperature drop across each insulating layer, ideally, is proportional to the temperature drop across the test specimen times the ratio of the thermal conductance of the specimen to the insulating layer; thus, if the insulating layer is thin and has a relatively high thermal conductivity, the temperature drop across each insulating layer will be a very small fraction of the temperature drop across the test specimen. If the heat flux to the guard heater is the same as that to the meter heater, that is, there are no significant heat losses from the outer edge of the guard plate, the temperature in the heater core region essentially will be the same for the guard plate as it is for the meter plate. In such a case, controlling the power input to the guard plate so that the gap thermopile gives a null output, not only will result in the temperatures of the surface plates

being identical but also will result in a temperature balance between the meter and guard plates.

X2.5.3 Single-Sided Mode—In this example, the two heaters are part of a single winding and cannot be operated separately. When operated in a single-sided mode, half of the heat flow through the test specimen comes from the heater on the front side of the guarded hot plate, half from the backside heater. The second temperature profile shown in Fig. X2.2b illustrates the variation in spatially averaged temperature through the guarded hot plate when operated in the single-sided mode with the same heat flux through the test specimen as above (X2.5.2). The temperature drop across the insulating layer on the front side is the same as it was in the double-sided mode, since the total heat flow through that layer is the same in each case; however, the heat flow from the heater on the backside of the hot plate shall pass through the heater core region, resulting in a significant temperature drop. In drawing this curve, it is assumed that the surface temperature of the auxiliary cold plate is the same as the surface temperature of the backside of the guarded hot plate so that there is no heat flow through the auxiliary insulation and no temperature gradient through the insulating layer behind the heater on the backside of the hot plate. In some guarded hot plate designs, the heater core is thick enough, and its thermal conductivity low enough, that the temperature drop, $T_h' - T_h$, across the guarded hot plate is a significant fraction of the temperature drop across the test specimen. Under such conditions, and depending on the thermopile installation, controlling the guard heater so that the thermopile produces a null output does not ensure that, in fact, there is a temperature balance between the meter and guard plates. In this case, significant errors occur in the determination of the heat flow through the test specimen due to extraneous heat flows across the gap or across the portions of the test specimen or the auxiliary specimen in the proximity of the gap.

X2.6 For a guarded-hot-plate apparatus that is capable of operation in both the double- and single-sided mode, the significance of errors in the gap heat flow is determined by conducting measurements on the same specimens in both

modes of operation, preferably with the same hot-side and cold-side temperatures in both modes of testing. The average conductance of a matched pair of specimens shall be determined by operating the apparatus in the double-sided mode. The average conductance of this pair of specimens also shall be determined from data taken on each specimen in the single-sided mode of operation. It is recommended that such measurements be carried out on several thicknesses of each of several materials, representing the ranges of thermal conductances and thermal conductivities of interest.

NOTE X2.3—The temperature variations in the portions of the guarded hot plate near the gap will depend primarily on the total heat flow required for the test, and hence, on the thermal conductance of the test specimen. For a given specimen thermal conductance, the extraneous heat flows through the portions of the test and auxiliary specimens adjacent to the gap will depend on the thermal conductivities of these specimens; thus, if there is a significant gap error, it probably will depend upon both the thermal conductances and the thermal conductivity of the test specimen.

X2.7 For a guarded-hot-plate apparatus that is only capable of operation in the single-sided mode, measurements are conducted on specimens whose thermal conductance is accurately known from measurements made in another guarded hot plate apparatus, or preferably, from a national standards laboratory. Such measurements shall be conducted on several thicknesses of several materials, representing the ranges of thermal conductances and thermal conductivities of interest.

X2.8 The differences between test data obtained using a single-sided mode of operation and the known thermal conductances obtained using a double-sided mode of operation or obtained in another guarded-hot-plate apparatus are analyzed to determine the magnitude of gap error, and if enough data are available, its dependence upon the thermal conductance and thermal conductivity of the test specimen. If a significant gap error is found, further analysis of the particular guarded-hot-plate design shall be carried out in order to predict the error for other specimen conductances and conductivities. If the error is very large or if reliable corrections cannot be made, the design of the gap thermopile, or even of the guarded hot plate itself, shall be changed.

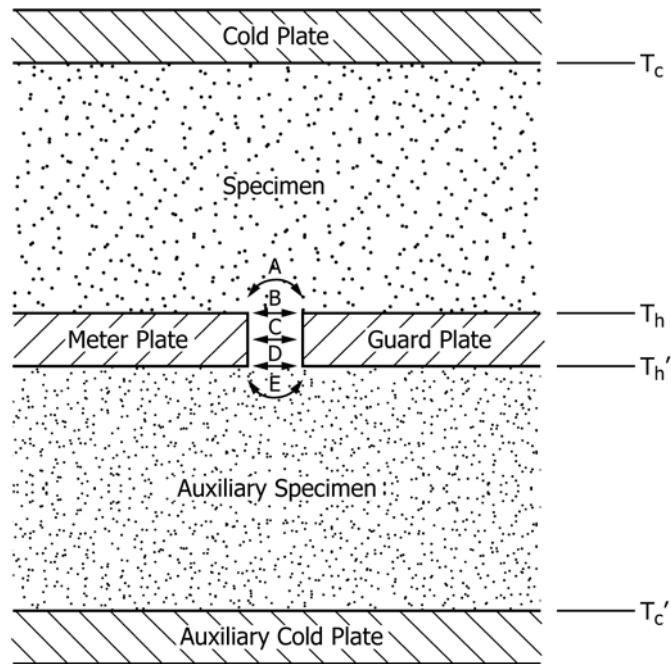


FIG. X2.1 Diagram Illustrating Heat Flows at Gap Region

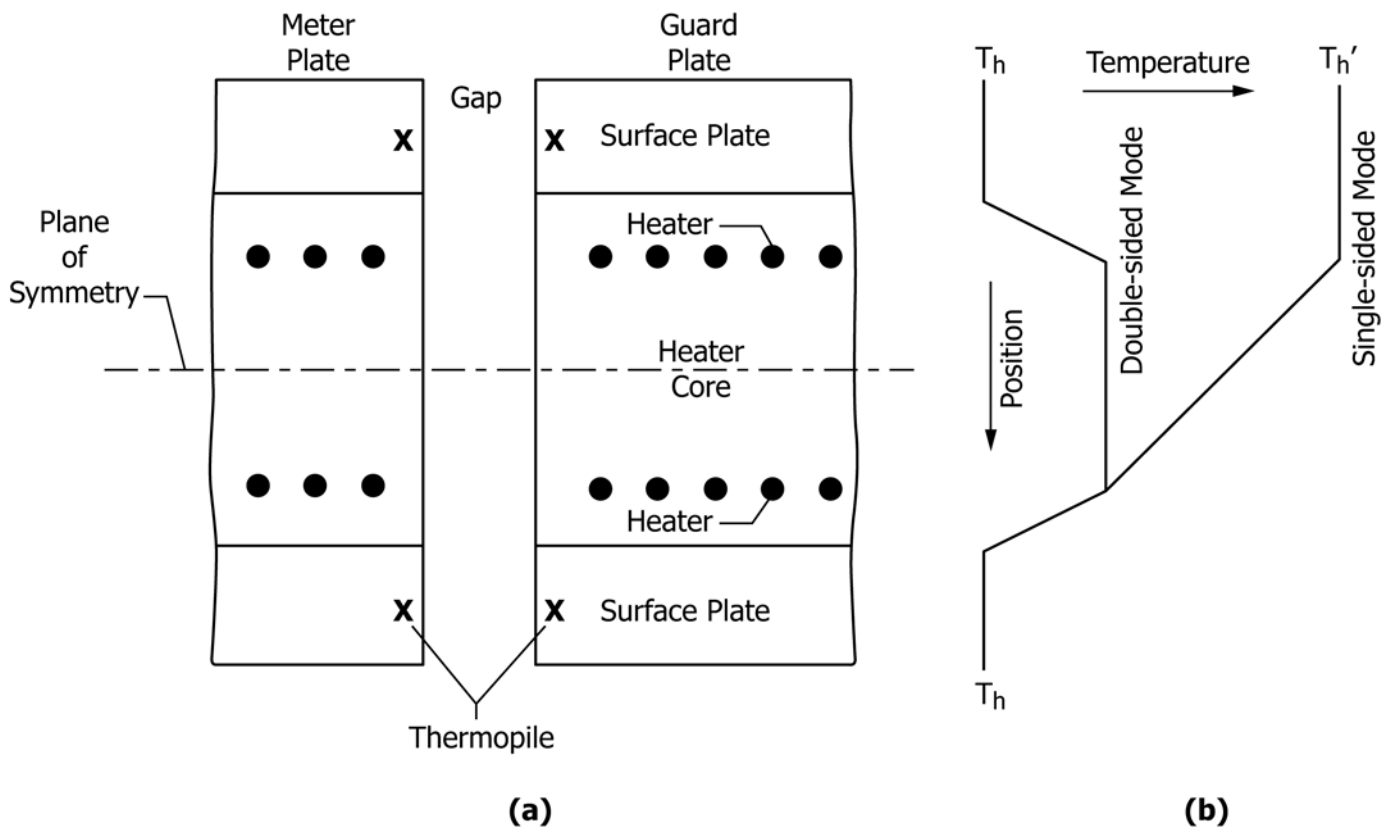


FIG. X2.2 Diagram of (Hypothetical) Guarded-Hot-Plate with Distributed Heat Source, and (b) Corresponding Temperature Profile for Double- and Single-sided Mode of Operation

X3. COMMENTARY

X3.1 *Introduction and History of Practice C1045:*

X3.1.1 This commentary provides the user with the background and history of this practice. It includes a brief discussion on the precision and bias of using either a guarded-hot-plate apparatus or a thin-heater apparatus in the single-sided mode of operation.

X3.1.2 The guarded-hot-plate apparatus and thin-heater apparatus traditionally have been operated in a double-sided mode of operation. The double-sided mode of operation requires similar specimens placed on either side of the hot plate. The two cold plates that contact the outer surfaces of these specimens are maintained at essentially the same temperature. The electric power supplied to the meter plate is assumed to result in equal heat flow through the meter section of each specimen so that the thermal transmission properties correspond to an average for the two specimens.

X3.1.3 For the single-sided mode of operation, a single specimen is placed between the hot plate and the cold plate. Auxiliary thermal insulation is placed between the hot plate and the auxiliary cold plate, that is, the other cold plate. The auxiliary cold plate and the hot plate are maintained at essentially the same temperature, which requires that each cold plate have separate temperature controls. Ideally, the heat flow from the meter plate is assumed to flow only through the specimen so that the thermal transmission properties correspond only to the specimen.

X3.1.4 In recent years, the single-sided practice has obtained favorable acceptance among several laboratories. The practice is employed frequently when only one specimen is available, for example, a loose-fill specimen prepared by pneumatic application. Further, the practice is required for the

preparation of calibrated transfer specimens for use with Test Method C518. The practice also is used for other research proposes, such as checking the homogeneity of stock material or determining the onset of convection in a specimen.

X3.1.5 In 1985, the practice for using the guarded-hot-plate apparatus in the one-sided mode was adopted by ASTM with a minor revision made in 1989. In 1998, this practice was revised extensively with changes in title and scope with a minor revision made in 2007. In 2012, this practice was revised with a discussion on measurement uncertainty. In 2016, this practice was revised for the use of mandatory language.

X3.2 *Precision and Bias:*

X3.2.1 Statements on precision and bias for guard-hot-plate apparatus and thin-heater apparatus are covered in Test Methods C177 and C1114, respectively. Currently, the statements do not distinguish between double-sided or single-sided operation. The user is directed instead to the theoretical treatment and interlaboratory tests reported below if information on precision and bias is required.

X3.2.2 A theoretical error analysis for a circular guarded-hot-plate apparatus operated in the single sided mode is discussed by Eguchi (4).

X3.2.3 *Interlaboratory Tests*—In 1993, an interlaboratory comparison that involved laboratories with guarded hot plate operated in either double- or single-sided operation was published (5).

X3.3 *Measurement Uncertainty:*

X3.3.1 Guidance on the determination of the measurement uncertainty for the single-sided mode of operation, is provided in (6).

REFERENCES

- (1) Pratt, A.W., "Heat Transmission in Low Conductivity Materials," Chapter 6 in *Thermal Conductivity*, Vol 1, R.P. Tye, Ed., New York, NY: Academic Press Inc., 1969, pp. 338-357.
- (2) Peavy, B. and Rennex, B.G., "Circular and Square Edge Effects Study for Guarded-Hot-Plate and Heat-Flow-Meter Apparatuses," *Journal of Thermal Insulation*, Vol 9, April 1986, pp. 254-300.
- (3) Ku, H.H., "Notes on the Use of Propagation of Error Formulas," *Journal of Research of the National Bureau of Standards*, Vol 70C, No. 4, October-November 1966.
- (4) Eguchi, K., "Error Analysis of Measuring Thermal Conductivity by Circular and One Side Heat Flow Type Guarded-Hot-Plate Apparatus," *ASTM STP 879*, ASTM, 1985, pp. 49-68.
- (5) Salmon, D., Silberstein, A., and Kumaran, K., "Report on Interlaboratory Comparison of Guarded-Hot-Plate Measurements," *National Research Council Canada Internal Report No. 653*, December 1993.
- (6) Zarr, R.R., "Assessment of Uncertainties for the NIST 1016 mm Guarded-Hot-Plate Apparatus: Extended Analysis for Low Density Fibrous-Glass Thermal Insulation," *Journal of Research of The National Institute of Standards and Technology*, 115, 23-59, 2010.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>