



Standard Test Method for Nickel on Steel for Porcelain Enameling by Photometric Analysis¹

This standard is issued under the fixed designation C715; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

INTRODUCTION

The test is designed to give a sufficiently accurate and rapid test of the amount of nickel deposited on sheet steel for enameling plant control work via a photometric method. However, the approximations used in the method prevent its use where extremely accurate nickel determinations are required. The method is applicable to control the weight of nickel coating on the metal.

1. Scope

1.1 This test method covers the determination of the amount of nickel deposited on sheet steel during its preparation for porcelain enameling. It is a photometric method commonly used on production parts and is suitable for determining the heavier nickel deposits that may be obtained during the processing of steel for one-coat enameling.

NOTE 1—An alternative X-ray emission spectrometry method is Test Method C810.

1.2 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:²

C810 Test Method for Nickel on Steel for Porcelain Enameling by X-Ray Emission Spectrometry

E30 Test Methods for Chemical Analysis of Steel, Cast Iron, Open-Hearth Iron, and Wrought Iron (Withdrawn 1995)³

E60 Practice for Analysis of Metals, Ores, and Related Materials by Spectrophotometry

¹ This test method is under the jurisdiction of ASTM Committee B08 on Metallic and Inorganic Coatings and is the direct responsibility of Subcommittee B08.12 on Materials for Porcelain Enamel and Ceramic-Metal Systems.

Current edition approved Nov. 1, 2016. Published November 2016. Originally approved in 1977. Last previous edition approved in 2011 as C715 – 90 (2011) ^{ϵ 1}. DOI: 10.1520/C0715-90R16.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ The last approved version of this historical standard is referenced on www.astm.org.

3. Significance and Use

3.1 This test method is primarily used to control the nickel dipping operation to ensure that the desired level of nickel deposition is attained. It is also used to prepare test plates used for calibration in Test Method C810.

4. Apparatus

4.1 *Photoelectric Photometer*, conforming to Practice E60.


4.2 *Weighted Rubber Ring Assembly*, required to confine stripping agents to a definite area, consisting of a molded rubber ring and a metal outer ring. The rubber ring shall have an inside diameter of 1.35 in. (34.3 mm) in order to encircle an area of 0.01 ft² (0.000929 m²), a wall configuration as shown in Fig. 1, and the lower portion beveled at a 45° angle (0.78 rad) to reduce the contact area and ensure a better seal. The metal outer ring shall weigh about 3.5 lb (1.5 kg), suitably machined to fit over the top of the rubber ring as shown in Fig. 1.

4.2.1 The exact area covered by the rubber ring will gradually increase as the rubber ring itself is consumed by the acid reagent used. In the most accurate analysis, the area etched by the rubber ring shall be calculated occasionally, factored against the prescribed area, and that number applied to the reading obtained from the graph.

4.3 *Aspirator*, consisting of a calibrated 500-mL flask, equipped with a twohole stopper, an aspirator bulb, and a suction tube formed from 0.079-in. (2-mm) inside diameter capillary glass tubing.

5. Reagents and Materials

5.1 Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee of Analytical

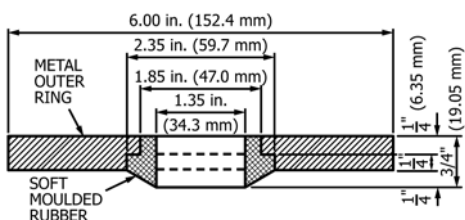

NOTE 1—The outer ring is a steel disk approximately 6 by 1/2 in. (152 by 13 mm), weighing approximately 3 1/2 lb (1.58 kg).

FIG. 1 Detailed Drawing of Rubber Ring

Reagents of the American Chemical Society.⁴ Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

5.2 *Purity of Water*—Use distilled or deionized water.

5.3 *Ammonium Hydroxide (sp gr 0.90)*—Concentrated ammonium hydroxide (NH₄OH).

5.4 *Ammonium Persulfate*—(NH₄)₂S₂O₈.

5.5 *Dimethylglyoxime*—Prepare a 1 % solution of dimethylglyoxime in methyl alcohol or a 2.62 % solution of sodium dimethylglyoximate in water (store in a polyethylene bottle).

5.6 *Hydrochloric Acid (1+5)*—Dilute 1 vol of concentrated hydrochloric acid (HCl, sp gr 1.19) with 5 vol of water.

5.7 *Nickel Sulfate, Standard Solution*—Dissolve 0.448 g of nickel sulfate (NiSO₄·6H₂O) in water. When the material is completely dissolved, cautiously add 10 mL of concentrated H₂SO₄ and transfer the solution to the 1000-mL flask. When cool, make up to the mark with water. One millilitre of this standard solution is equivalent to 0.0001 g of nickel per millilitre.

5.8 *Nitric Acid (1+1)*—Dilute 1 vol of concentrated nitric acid (HNO₃, sp gr 1.42) with 1 vol of water.

5.9 *Sulfuric Acid (sp gr 1.84)*—Concentrated sulfuric acid (H₂SO₄).

6. Sampling

6.1 Sampling frequency shall be consistent with the objective of control of the nickel dipping operation.

7. Standardization of Photoelectric Photometer

7.1 The photoelectric photometer shall be standardized as follows:

7.1.1 Using a buret, accurately measure out 2, 4, 8, 12, 16, and 20 mL portions of nickel sulfate standard solution. These amounts are equivalent to 0.2, 0.4, 0.9, 1.3, 1.7, and 2.1 g of nickel per square metre (0.02, 0.04, 0.08, 0.12, 0.16, and 0.20 g of nickel per square foot) of surface when specimens from the steel surface are obtained as prescribed. (Iron in solution

that is dissolved from the steel surfaces has a negligible effect on the nickel determinations.) Using the standard analytical procedures described in 8.2, determine the percent transmission at a wavelength of approximately 525 nm for each of the six increments of nickel sulfate standard solution. Then plot a graph on appropriate graph paper of the percent light transmission against the known nickel concentration representing 0.2 to 2.1 g of nickel deposit per square metre of surface. The resulting graph, which should be a straight line, will be used to obtain nickel-coating masses from light transmission results.

8. Determinations of Nickel Coating Masses

8.1 Sampling a Nickel-Coated Steel Surface:

8.1.1 Place the weighted, rubber ring assembly on the nickel-coated metal surface. Add 3 mL of warm (approximately 120°F (50°C)) HNO₃ (1+1). Allow the foaming reaction to proceed for about 10 s for light nickel coatings and about 15 s for heavier nickel coatings. If the warm acid does not react, scratch the steel surface or try another spot. After the acid has foamed for the prescribed time, add 5 mL of HCl (1+5) to stop the foaming reaction. Withdraw the solution from the steel surface with the aspirator into the calibrated flask. Rinse the test area twice with water and retain the washings in the flask.

8.1.2 Alternative methods for determining nickel are described in Test Methods E30, Sections 62 to 70 for the gravimetric method and Sections 71 to 73 for the volumetric method.

8.2 Analytical Procedure:

8.2.1 Add chemicals in the order given below to the solution in the flask and mix thoroughly after each addition:

Additions for 23-mm Optical Path Cell ^A	Amount in Order of Use
Ammonium hydroxide (sp gr 0.90)	50 mL
Ammonium persulfate	4 g
Dimethylglyoxime	10 mL
Dilute with water to	500 mL

^A Cells with other optical path lengths are available.

8.2.2 Filter a portion of the solution. Discard the first 10 to 20 mL from the filter and collect a sufficient amount of filtrate in the absorption cell for testing. Just before testing, set the wavelength as determined in accordance with Section 7 and adjust the instrument to 100 % transmission with a cell that contains only water. Place the cell containing the test solution in the photometer and read the percent transmission.

9. Calculation and Report

9.1 Refer to the graph developed in Section 7. Determine the mass of nickel that corresponds to the percent transmission reading shown by the photometer. Report the results in grams of nickel per square metre of steel surface.

10. Precision and Bias

10.1 The precision and bias of this test method is believed to be within 0.000929 g/ft² (0.1 g/m²). Exact values are difficult to obtain because of sample inhomogeneity, and the effect of the acid etch on the rubber ring diameter (see 4.2.1).

⁴ Reagent Chemicals, American Chemical Society Specifications, American Chemical Society, Washington, DC. For suggestions on the testing of reagents not listed by the American Chemical Society, see *Analar Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>