



Standard Test Methods for Density of Soil and Rock in Place by the Sand Replacement Method in a Test Pit¹

This standard is issued under the fixed designation D4914/D4914M; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

1. Scope*

1.1 These test methods cover the determination of the in-place density of soil and rock using a pouring device and calibrated sand to determine the volume of a test pit. The word “rock” in these test methods is used to imply that the material being tested will typically contain particles larger than 3 in. [75 mm].

1.2 These test methods are best suited for test pits with a volume from 0.03 to 0.17 m³ [1 to 6 ft³]. In general, the materials tested would have a maximum particle size of 75 to 125 mm [3 to 5 in.].

1.2.1 For larger sized excavations and soil containing larger particles, Test Method D5030 is preferred.

1.2.2 Test Method D1556 or D2167 are usually used to determine the volume of test holes smaller than 0.03 m³ [1 ft³]. While the equipment illustrated in these test methods is used for volumes less than 0.03 m³ [1 ft³], the test methods allow larger versions of the equipment to be used when necessary.

1.3 Two test methods are provided as follows:

1.3.1 *Test Method A—In-Place Density of Total Material* (Section 10).

1.3.2 *Test Method B—In-Place Density of Control Fraction* (Section 11).

1.4 *Selection of Test Methods:*

1.4.1 Test Method A is used when the in-place density of total material is to be determined. Test Method A can also be used to determine percent compaction or percent relative density when the maximum particle size present in the in-place material being tested does not exceed the maximum particle size allowed in the laboratory compaction test (refer to Test Methods D698, D1557, D4253, D4254, and D7382). For Test Methods D698 and D1557 only, the dry density determined in the laboratory compaction test may be corrected for larger particle sizes in accordance with, and subject to the limitations of Practice D4718.

1.4.2 Test Method B is used when percent compaction or percent relative density is to be determined and the in-place material contains particles larger than the maximum particle size allowed in the laboratory compaction test or when Practice D4718 is not applicable for the laboratory compaction test. Then the material is considered to consist of two fractions, or portions. The material from the in-place dry density test is physically divided into a control fraction and an oversize fraction based on a designated sieve size (see Section 3). The dry density of the control fraction is calculated and compared with the dry density(s) established by the laboratory compaction test(s).

1.5 Any materials that can be excavated with hand tools can be tested provided that the void or pore openings in the mass are small enough (or a liner is used) to prevent the calibrated sand used in the test from entering the natural voids. The material being tested should have sufficient cohesion or particle interlocking to maintain stable sides during excavation of the test pit and through completion of this test. It should also be firm enough not to deform or slough due to the minor pressures exerted in digging the hole and pouring the sand.

1.6 These test methods are generally limited to material in an unsaturated condition and are not recommended for materials that are soft or friable (crumble easily) or in a water condition such that water seeps into the hand-excavated hole. The accuracy of the test methods may be affected for materials that deform easily or that may undergo volume change in the excavated hole from standing or walking near the hole during the test.

1.7 The values stated in either SI units or inch-pound presented in brackets are to be regarded separately as standard. The values stated in each system may not be exact equivalents; therefore each system shall be used independently of the other. Combining values from the two systems may result in non-conformance with the standard.

1.8 All observed and calculated values shall conform to the guidelines for significant digits and rounding established in Practice D6026.

1.8.1 The procedures used to specify how data are collected, recorded or calculated in this standard are regarded as the industry standard. In addition they are representative of the

¹ These test methods are under the jurisdiction of ASTM Committee D18 on Soil and Rock and are the direct responsibility of Subcommittee D18.08 on Special and Construction Control Tests.

Current edition approved March 1, 2016. Published March 2016. Originally approved in 1989. Last previous edition approved in 2008 as D4914 – 08. DOI: 10.1520/D4914_D4914M-16.



significant digits that generally should be retained. The procedures used do not consider material variation, purpose for obtaining the data, special purpose studies, or any considerations for the user's objectives; it is common practice to increase or reduce significant digits of reported data to be commensurate with these considerations. It is beyond the scope of this standard to consider significant digits used in analytical methods for engineering design.

1.9 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* For specific hazards statements, see Sections 8 and A1.5.

2. Referenced Documents

2.1 ASTM Standards:²

- C127 Test Method for Relative Density (Specific Gravity) and Absorption of Coarse Aggregate
- C566 Test Method for Total Evaporable Moisture Content of Aggregate by Drying
- D653 Terminology Relating to Soil, Rock, and Contained Fluids
- D698 Test Methods for Laboratory Compaction Characteristics of Soil Using Standard Effort (12 400 ft-lbf/ft³ (600 kN-m/m³))
- D1556 Test Method for Density and Unit Weight of Soil in Place by Sand-Cone Method
- D1557 Test Methods for Laboratory Compaction Characteristics of Soil Using Modified Effort (56,000 ft-lbf/ft³ (2,700 kN-m/m³))
- D2167 Test Method for Density and Unit Weight of Soil in Place by the Rubber Balloon Method
- D2216 Test Methods for Laboratory Determination of Water (Moisture) Content of Soil and Rock by Mass
- D3740 Practice for Minimum Requirements for Agencies Engaged in Testing and/or Inspection of Soil and Rock as Used in Engineering Design and Construction
- D4253 Test Methods for Maximum Index Density and Unit Weight of Soils Using a Vibratory Table
- D4254 Test Methods for Minimum Index Density and Unit Weight of Soils and Calculation of Relative Density
- D4718 Practice for Correction of Unit Weight and Water Content for Soils Containing Oversize Particles
- D4753 Guide for Evaluating, Selecting, and Specifying Balances and Standard Masses for Use in Soil, Rock, and Construction Materials Testing
- D5030 Test Method for Density of Soil and Rock in Place by the Water Replacement Method in a Test Pit
- D6026 Practice for Using Significant Digits in Geotechnical Data
- D7382 Test Methods for Determination of Maximum Dry Unit Weight and Water Content Range for Effective

Compaction of Granular Soils Using a Vibrating Hammer
E11 Specification for Woven Wire Test Sieve Cloth and Test Sieves

3. Terminology

3.1 Definitions:

3.1.1 For definitions of terms related to this standard, refer to Terminology D653.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *control fraction, n*—the portion of a soil sample consisting of particles smaller than a designated sieve size.

3.2.1.1 *Discussion*—This fraction is used to compare in-place density with density obtained from standard laboratory tests. The control sieve size depends on the laboratory test used. Normally, the control fraction is the minus 4.75 mm, or No. 4 [0.187 in.] sieve size material for cohesive or non-free draining materials and the minus 75 mm [3-in.] sieve size material for cohesionless, free-draining materials. While other sizes are used for the control fraction, 9.5 or 19 mm [$\frac{3}{8}$, $\frac{3}{4}$ -in.], these test methods have been prepared using only the No. 4 and the 75 mm [3 in.] sieve sizes for clarity.

3.2.2 *oversize particles, n*—the portion of a soil sample consisting of the particles larger than the designated sieve size for the control fraction selected.

3.2.3 *sand pouring device(s), n*—handheld pouring device(s) that holds the density sand equipped with a long pouring spout for placing the sand with unobstructed flow at a constant drop height.

3.2.3.1 *Discussion*—Multiple cans may be used but they must be of the same design and calibrated.

4. Summary of Test Method

4.1 The ground surface at the test location is prepared and a template (metal frame) is placed and fixed into position. The volume of the space between the top of the template and the ground surface is determined by filling the space with calibrated sand using a pouring device. The mass of the sand required to fill the template in place is determined and the sand removed. Material from within the boundaries of the template is excavated forming a pit. Calibrated sand is then poured into the pit and template; the mass of sand within the pit and the volume of the hole are determined. The wet density of the in-place material is calculated from the mass of material removed and the measured volume of the test pit. The water content is determined and the dry density of the in-place material is calculated.

4.2 The density of a control fraction of the material can be determined by subtracting the mass and volume of any oversize particles from the initial values and recalculating the density.

5. Significance and Use

5.1 These test methods are used to determine the in-place density of compacted materials in construction of earth embankments, road fills, and structure backfill. For construction control, these test methods are often used as the bases for acceptance of material compacted to a specified density or to a percentage of a maximum unit weight determined by a

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

standard laboratory test method (such as determined from Test Method **D698** or **D1557**), subject to the limitations discussed in 1.4.

5.2 These test methods can be used to determine the in-place density of natural soil deposits, aggregates, soil mixtures, or other similar material.

NOTE 1—The quality of the result produced by this standard is dependent on the competence of the personnel performing it, and the suitability of the equipment and facilities used. Agencies that meet the criteria of Practice **D3740** are generally considered capable of competent and objective testing. Users of these test methods are cautioned that compliance with Practice **D3740** does not in itself ensure reliable results. Reliable testing depends on many factors; Practice **D3740** provides a means of evaluating some of those factors.

6. Interferences

6.1 Because of possible lower densities created when there is particle interference (see Practice **D4718**), the percent compaction of the control fraction should not be assumed to represent the percent compaction of the total material in the field when using method B with oversize corrections.

6.2 A careful assessment must be made as to whether or not the volume determined is representative of the in-place condition when this test method is used for clean, relatively uniform-sized particles. The disturbance during excavation, due to lack of cohesion, and the void spaces between particles spanned by the liner (if used) may affect the measurement of the volume of the test pit.

NOTE 2—Experience with this test used in cohesionless uniform fine gravels, pea gravels, or processed uniform gravel drain materials have shown errors in test hole volume.

7. Apparatus

7.1 *Balance or Scale*—A balance (or scale) to determine the mass of the calibrated sand and the excavated soil having a minimum capacity of 20 kg [50 lbm] and meeting the requirements of Specification **D4753** for a balance of 1-g [0.002-lbm] readability.

7.2 *Balance or Scale*—A balance (or scale) to determine water content of minus No. 4 material having a minimum capacity of 1000 g [2-lbm] and meeting the requirements of Specification **D4753** for a balance of 0.1 g [0.001 lbm] readability.

7.3 *Drying Oven*—An oven, thermostatically controlled, preferably of the forced-draft type, and capable of maintaining a uniform temperature of $110 \pm 5^\circ\text{C}$ throughout the drying chamber.

7.4 *Sieves*—No. 4, 4.75-mm [0.187-in.] sieve and 75-mm [3-in.] sieve, conforming to the requirements of Specification **E11**.

7.5 *Metal Template*—A square or circular template to serve as a pattern for the excavation. Template dimensions, shapes, and material may vary according to the size of the test pit to be excavated. Refer to **Appendix X1** for recommended template sizes. The template shall be rigid enough not to deflect or bend.

NOTE 3—The template shown in **Fig. 1** represents a design that has been found suitable for this purpose.

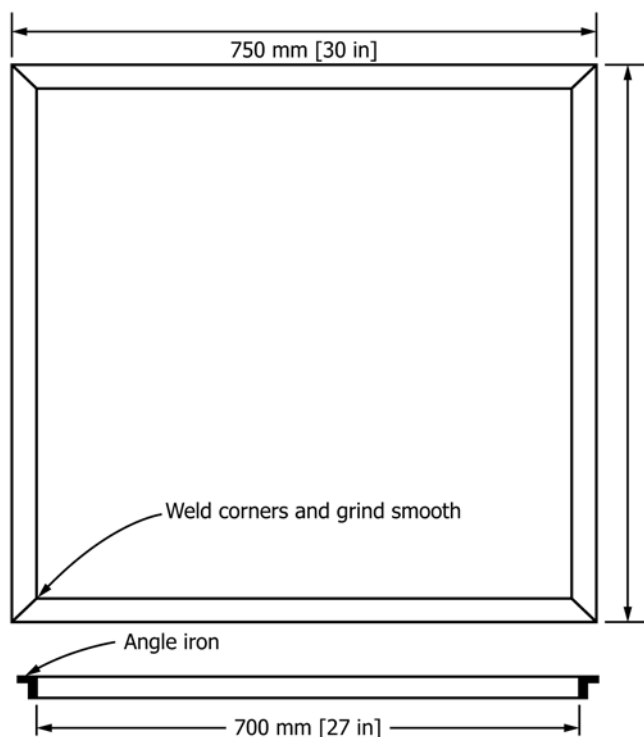


FIG. 1 Typical Metal Template for Excavating Test Pit

7.6 *Liner*, approximately less than 25 μm [1 mil, 0.001 in.] thick and large enough to line the test pit with about 0.3 m [1 ft] extending beyond the outside of the template. Any type of material, plastic sheeting, etc., can be used as long as it is flexible enough to conform to the ground surface.

7.7 *Sand Pouring Devices*—(See **Fig. 2** for some typical devices.) Many types of pouring devices are available. Use multiple 10 to 15-L [3 to 4-gal] containers as long as they meet spout requirements. Larger containers may be used as long as the vertical 50-mm [2-in.] drop height can be maintained. The device must have a spout that will reach into a field test pit so that the drop distance from the end of the spout to the sand surface can be maintained at about 50 mm [2 in.]. The inside diameter of the spout must also be large enough to allow free flow of the sand without clogging.

7.8 *Metal Straightedge*, about 50 mm [2 in.] high, at least 3 mm [$\frac{1}{8}$ in.] thick, and with a length 1.5 times the side length (or diameter) of the metal template, used for screeding excess sand placed in template. It must have a thickness or rigidity such that it will not bend when screeding the sand.

7.9 *Sand*—The sand must be clean, dry, uniform, uncemented, durable, and free flowing. The gradation, physical characteristics, selection, and storage of the sand shall meet the requirements of Test Method **D1556** except that the maximum particle size may be No. 4, 4.75-mm [0.187-in.] sieve.

7.9.1 If the test methods are used for test pits larger than about 0.2 m^3 [6 ft^3], a one-size material relatively free of fines and of a larger particle size, such as pea gravel, may be used.

7.10 *Miscellaneous Equipment*—Shovels for preparing test surface; hammer for seating template; assorted small brushes,

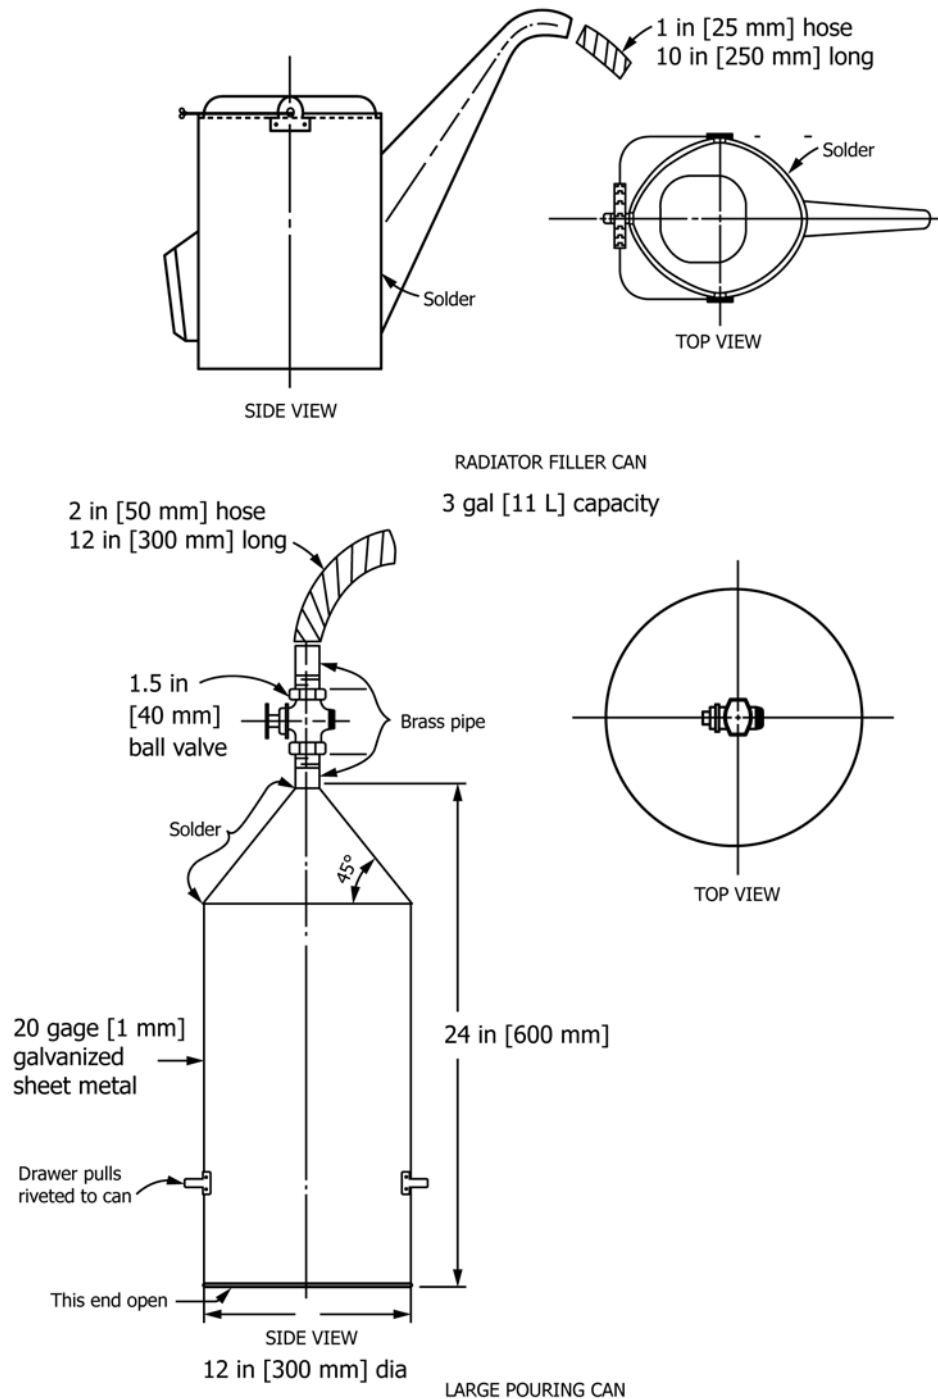


FIG. 2 Typical Sand Pouring Devices (Dimensions in Inches with Rationalized SI Equivalent)

picks, chisels, bars, knives, and spoons for digging test pit; buckets with lids, seamless cans with lids, or other suitable containers for retaining the test sample and sand without water content change; bags or other suitable containers for waste sand; cloth for collecting excess sand or soil; and assorted pans and porcelain dishes suitable for drying water content specimens.

8. Hazards

8.1 Precaution:

8.1.1 These test methods may involve handling heavy loads.

8.1.2 Some sands used in the procedures outlined herein may be dusty and appropriate precautions should be taken when mixing and pouring. Use dust masks during sand pouring operations to avoid inhalation of silica dust.

8.2 Caution:

8.2.1 Materials that may flow or deform during the test must be identified and appropriate precautions taken.

8.2.2 Movement of heavy equipment in the immediate test area should not be permitted during the volume determination.



8.2.3 Errors may arise in the computed density of material due to the influence of excessive water in the soil. These errors may be significant in materials with high permeability, such as sands and gravels, where the bottom of the test hole is close to or below the water table. Errors may also arise due to change in density of the calibrated sand as it becomes wetted from capillary or freestanding water while performing the test. This problem becomes evident when removing the calibrated sand from the test hole and wet sand is observed on the bottom or sides of the test hole. When a liner is used, the buoyant forces of free water beneath or behind the liner may adversely affect the volume determination.

8.2.4 Suitably protect the test area and equipment during periods of inclement weather such as rain, snowfall, or high wind. If the in-place water content value is required, it may be necessary to protect the area from direct sunlight.

8.2.5 Numerous containers may be required during performance of these test methods. Properly label all containers to avoid a possible mix-up.

8.2.6 The total mass of the calibrated sand, or the soil sample, or both, may exceed the capacity of the scale used, requiring cumulative determinations of mass. Take care to ensure that the total mass is properly determined.

8.2.7 Pouring devices with valves provide consistent sand flow from test to test only if the valve is opened completely each time. A valve that is only partially open can significantly alter the flow characteristics of the device. Each individual pouring device has unique characteristics which may cause the sand to flow from it differently. The final calibration values are affected by changes in these flow characteristics. Consequently, calibration values are not interchangeable, even for devices which may appear to be identical.

8.2.8 Do not allow pouring devices to run out of sand during the pouring operation. The size of the stream of poured sand from the pouring device should be constant. If the reservoir capacity of the pouring device is too small to fill the test pit with one pour, use two or more pours to fill the test pit. Stop the stream of sand when the reservoir is about three-fourths empty and before the size of the stream diminishes. Refill the reservoir and resume pouring.

8.2.9 Pouring devices permit a varied sand drop distance that must be carefully controlled if consistent results are to be achieved. A distance of 50 mm [2 in.] from the end of the spout to the surface being poured is recommended. Variations in the drop distance can significantly affect results. The drop distance is directly affected by the operator's ability to control the pouring device and by the operator's judgment of the drop distance while doing so. This involves stooping while holding a pouring device with an initial mass of 20 kg [50 lbm] or more that is constantly changing in mass as the sand flows into the test pit. Calibration values are not interchangeable from device to device and are not necessarily interchangeable from operator to operator. Individual operators must demonstrate that they can duplicate the calibration values for a device before they may use them, preferably within 1 % of the average value for another operator. Otherwise, separate calibrations for the various operators are required.

9. Calibration and Standardization

9.1 Calibrate the sand pouring equipment and sand in accordance with [Annex A1](#).

10. Test Method A, Procedure—In-Place Density of Total Material

10.1 Use Test Method A to determine a total in-place density (see [1.4](#)).

10.2 Determine the recommended sample volume and select the appropriate template for the anticipated material gradation in accordance with [Annex A2](#). Assemble the remainder of the required equipment.

10.3 Determine the mass of each combination of empty container, lid, and container liner (if used) that will contain the excavated material. Number the containers and mark as to use. Write the mass on the container or prepare a separate list.

10.4 Prepare the quantity of calibrated sand to be used.

10.4.1 Two sets of calibrated sand are necessary. Determining the volume of the test pit requires two separate sand pours to (1) measure the mass of sand used to fill the space between the soil surface and the top of the template, and (2) measure the mass of sand used to fill the test pit up to the top of the template. The difference between the two gives the mass of sand in the test pit.

10.4.2 Estimate the mass of calibrated sand and the number of containers required to fill the space between the soil surface and the top of the template. Calculate the estimated mass by multiplying the template volume by the density of the calibrated sand. Number the containers to be used and mark as to use, for example, "template correction." Fill the containers with sand. Determine and record on a separate list the mass of the containers and sand.

10.4.3 From the anticipated volume of the test pit, estimate the mass of calibrated sand required to fill the test pit. Increase this amount by about 25 % to make sure that a sufficient sand supply is available at the site, and then add to it the mass of sand calculated in [10.4.2](#). Calculate the estimated mass to be used for the test pit by multiplying the anticipated volume of the test pit by the density of the calibrated sand. Determine the number of containers required, number them, and mark as to use, for example, "test pit." Fill the containers with sand. Determine and record on a separate list the mass of the containers and sand.

10.5 Select a representative area for the test, avoiding locations where removal of large particles would undermine the template.

10.6 Prepare the surface of the area to be tested.

10.6.1 Remove all loose material from an area large enough on which to place the template. Prepare the exposed surface so that it is a firm, level plane.

10.6.2 Personnel should not step on the area selected for testing. Provide a working platform when testing materials which may flow or deform.

10.7 Place and seat the template on the prepared surface.

10.7.1 Use a hammer to firmly seat the template to avoid movement of the template while the test is performed. The use of nails, weights, or other means may be necessary to maintain the position.

10.7.2 Remove any material loosened while placing and seating the template, taking care to avoid leaving any void space under the template. If necessary, fill voids under the template with plastic soil, modeling clay, or other suitable material, provided that this material is not subsequently excavated as part of the material removed from the test pit.

10.8 Determine the mass of sand used to fill the space between the soil surface and the top of the template.

10.8.1 Irregularities of the soil surface within the template must be taken into account. To do this, determine the mass of sand required to fill the space between the soil surface and the top of the template.

10.8.2 It is recommended that a cloth with a hole slightly larger than the template center hole be placed over the template to facilitate locating and collecting any excess sand, or loose material, or both.

10.8.3 Place a liner over the template and shape it by hand to conform to the irregular soil surface and the template. The liner should extend approximately 0.3 m [1 ft] outside the template. The liner should not be stretched too taut or contain excessive folds or wrinkles (see Fig. 3).

10.8.4 Pour the calibrated sand onto the liner inside the template using a sand pouring device (see Fig. 4). Slightly overfill the template (see 8.2.7 – 8.2.9). Return any sand remaining in the pouring device to the original container.

10.8.5 Carefully level the calibrated sand by screeding with the steel straightedge across the top edges of the template. Return all screeded excess sand to the original container. Take care to avoid the loss of any excess sand.

10.8.6 Remove the calibrated sand in the template and, if the sand is to be reclaimed, place it in a specially marked container. Remove the liner.

10.9 Excavate the test pit.

10.9.1 Using hand tools (chisel, knife, bar, etc.), excavate the center portion of the test pit.

10.9.1.1 Do not permit any movement of heavy equipment in the area of the test pit as deformation of the soil within the test pit may occur.



FIG. 4 Sand Being Poured Into the Template

10.9.2 Place all material removed from the test pit in the container(s) (see Fig. 5), being careful to avoid losing any material (see 10.8.2).

10.9.3 Avoid water loss by keeping the container covered while material is not being placed in it. Use a sealable plastic bag inside the container to hold the material.

10.9.4 Carefully trim the sides of the excavation so that the dimensions of the test pit at the soil-template contact are as close as possible to that of the template hole. Avoid disturbing the template or the material beneath or outside the template.

10.9.5 Continue the excavation to the required depth, carefully removing any material that has been compacted or loosened in the process.

10.9.5.1 If during excavation of material from within the test pit, a particle(s) is found that is about 1½ times, or more, larger than the maximum particle size used to establish the dimensions and minimum volume of the test pit (see Annex A2), set the particle(s) aside and mark appropriately. Determine the mass and volume of the particle(s) and then subtract them from the mass and volume of the material removed from the test pit. Consider the larger particle(s) as “oversize” and follow the procedure outlined in Section 11, except that the “total” density, which would include the larger particle(s), need not be calculated. The “control fraction” values determined then become the values for the total material from the test pit. If enough of these particles are found so that their mass is determined to be about 5 % or more of the mass of the excavated material, repeat the test with a larger test pit in accordance with the guidelines in Annex A2.

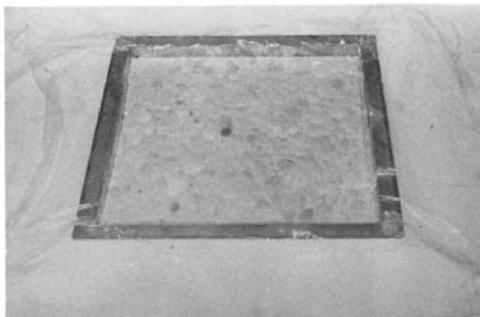


FIG. 3 Plastic Liner Placed Over the Template



FIG. 5 Excavation of the Test Pit

10.9.6 The sides of the pit should slope inward slightly. Materials that do not exhibit much cohesion may require a more conical-shaped test hole.

10.9.7 The profile of the finished pit must be such that poured sand will completely fill the excavation. The sides of the test pit should be as smooth as possible and free of pockets or overhangs or anything that might interfere with the free flow of the sand.

10.9.8 Clean the bottom of the test pit of all loosened material.

10.10 Determine the volume of the test pit.

NOTE 4—A liner may be required to prevent migration of the calibrated sand into the natural voids of the material mass. The liner, approximately ½-mil thick, should be large enough to extend approximately 0.3 m (1 ft) outside of the template after having been carefully placed and shaped to the soil surface within the pit. Allowances must be made for slack. The liner should not be stretched too taut nor contain excessive folds or wrinkles. Inspect the liner for punctures before use.

10.10.1 Pour the calibrated sand using the sand pouring device. Use the same pouring technique as used in the calibration procedure described in **Annex A1**. Slightly overfill the template. Return any sand remaining in the pouring device to the original container.

10.10.1.1 While the sand is being poured, avoid any vibrations in the test area.

10.10.2 Carefully level the calibrated sand by screeding with the steel straightedge across the top edges of the template. Return all screeded excess sand to the original container. Take care to avoid the loss of any excess sand.

10.10.3 If the calibrated sand is to be reclaimed, remove the used sand and place it into a specially marked container. Remove the liner and template.

10.11 Determine the dry density. Equations for calculations are shown in Section 12.

10.11.1 Determine the mass of calibrated sand in the template (sand used to fill the space between the soil surface and the top of the template) as follows:

10.11.1.1 Calculate and record the total mass of the sand and containers prepared in 10.4.2. Record the container numbers.

10.11.1.2 Determine and record the total mass of the empty containers plus the sand residue (sand not used) and containers.

10.11.1.3 Calculate the mass of sand in the template and record.

10.11.2 Determine the mass of calibrated sand in the test pit and template (sand used to fill the test pit to the top of the template) as follows:

10.11.2.1 Calculate and record the total mass of the sand and containers prepared in 10.4.3. Record the container numbers.

10.11.2.2 Determine the total mass of the empty containers plus the sand residue and containers and record.

10.11.2.3 Calculate the mass of sand in the test pit and template (mass of sand used) and record.

10.11.3 Calculate the mass of the calibrated sand used to fill the test pit and record.

10.11.4 Record the density of the calibrated sand (determined in the calibration procedure described in **Annex A1**).

10.11.5 Calculate the volume of the test pit and record.

10.11.6 Determine the total mass of the excavated material and containers.

10.11.7 Calculate and record the total mass of the containers used to hold the excavated material. Record the container numbers.

10.11.8 Calculate the mass of the excavated material and record.

10.11.9 Calculate the wet density of the excavated material.

10.11.10 If the excavated material contains oversize particles (normally larger than the 4.75-mm (No. 4) sieve for cohesive materials and 75-mm [3-in.] sieve for cohesionless materials), separate the material using the appropriate size sieve. If the material contains about 3 % (wet basis) or more oversize particles, Test Method B should be used.

10.11.11 If 2 % or less oversize particles are present, obtain a water content specimen representative of the excavated material and determine the water content in accordance with Test Method **D2216** or **C566** and record.

NOTE 5—For rapid water content determination of materials containing less than 15 % fines (minus No. 200), use a suitable source of heat such as an electric or gas hotplate. If a source of heat other than the controlled temperature oven is used, stir the test specimen to accelerate drying and avoid localized overheating. The material may be considered dry when further heating causes, or would cause, less than 0.1 % additional loss of mass.

10.11.12 Calculate and record the dry density of the material.

11. Test Method B, Procedure—In-Place Density of Control Fraction

11.1 This test method is used when the material being tested contains oversize particles and the percent compaction or percent relative density of the control fraction are to be determined (see 1.4).

11.2 Obtain the in-place wet density of total material by following the procedure for Test Method A, as stated in 10.1 – 10.11.9.

11.3 To obtain the wet density of the control fraction, determine the mass and volume of the oversize particles and subtract them from the total mass and total volume to get the mass and volume of the control fraction. Then calculate the density of the control fraction from the mass and volume of the control fraction. Equations for calculations are shown in Section 12.

11.3.1 Normally, the wet density of the control fraction is determined and the dry density calculated using the water content of the control fraction.

11.3.2 In addition, the water content of the oversize particles, the water content of the total material, and the percentage of oversize particles may be determined.

11.4 After obtaining the wet mass of total material removed from the test pit, separate the material into the control fraction and the oversize particles using the designated sieve. Do this rapidly to minimize loss of water. If the test is for construction control, place the control fraction in an airtight container for further tests.



11.5 Wash the oversize particles and reduce the free water on the surface of the particles by blotting, draining, or a similar method.

11.6 Determine the wet mass of the oversize particles plus a container of predetermined mass, and record.

11.7 Calculate the wet mass of the oversize particles and record.

11.8 Calculate the wet mass of the control fraction and record.

11.9 Determine the volume of the oversize particles by one of the following procedures:

11.9.1 Determine and record the mass of all oversize particles suspended in water using the procedures and principles of Test Method C127, disregarding the oven drying and 24-h soaking period. Calculate and record the volume of the oversize particles.

11.9.2 Calculate the volume of the oversize particles using a known bulk specific gravity value. If previous tests for bulk specific gravity of similar oversize particles from a particular source have been performed and the value is relatively constant, a bulk specific gravity may be assumed. The bulk specific gravity value used must correspond to the water condition of the oversize particles when their mass is determined. As used in this test method, determine the bulk specific gravity on the oversize particles in the water condition as stated in 11.5 – 11.7. If an oven dry or saturated surface dry (SSD) bulk specific gravity is used, then also determine the mass of the oversize particles for this test method on oven dry or SSD material, respectively.

11.10 Calculate the volume of the control fraction and record.

11.11 Calculate the wet density of the control fraction.

11.12 Determine the water content of the control fraction in accordance with Test Method D2216 or C566 (see Note 5) and record.

11.13 Calculate the dry density of the control fraction and record.

11.14 If desired, determine and record the water content of all oversize particles in accordance with Test Method D2216 or C566 (see Note 5). If previous tests for water content of the oversize particles from a particular source have been performed and the value is relatively constant, a water content may be assumed.

11.15 If desired, determine the percentage of oversize particles as follows:

11.15.1 Calculate the dry mass of the control fraction and record.

11.15.2 Calculate the dry mass of the oversize particles and record.

11.15.3 Calculate the dry mass of the total sample and record.

11.15.4 Calculate the percentage of oversize particles and record.

11.16 Calculate the water content of the total material.

11.17 Calculate the dry density of the total material and record.

12. Test Method A, Calculation

12.1 The calculations use units of kg and m³, for mass and volume calculation and then density is expressed in Mg/m³ using a conversion factor. Density can also be reported as kg/m³ without the conversion factor. Units of lbm and ft³ can also be substituted and used in the same equations for mass and volume and the density can be expressed in lbm/ft³.

12.2 Calculate the mass of the sand contained in the template as follows:

$$m_6 = m_2 - m_4 \quad (1)$$

where:

m_6 = mass of sand in template, kg,

m_2 = mass of template sand and container(s) (before test), kg, and

m_4 = mass of template sand residue and container(s) (after test), kg.

12.3 Calculate the mass of the sand used to fill the test pit and template as follows:

$$m_5 = m_1 - m_3 \quad (2)$$

where:

m_5 = mass of sand used, kg,

m_1 = mass of sand and container(s) (before test), kg, and

m_3 = mass of sand residue and container(s) (after test), kg.

12.4 Calculate the mass of the sand used to fill the test pit as follows:

$$m_7 = m_5 - m_6 \quad (3)$$

where:

m_7 = mass of sand in test pit, kg,

m_5 = mass of sand used, kg, and

m_6 = mass of sand in template, kg.

12.5 Calculate the volume of the test pit as follows:

$$V_T = \frac{m_7}{\rho_s} \times \frac{1}{10^3} \quad (4)$$

where:

V_T = volume of test pit, m³,

m_7 = mass of sand in test pit, kg, and

ρ_s = density of calibrated sand, Mg/m³.

12.6 Calculate the mass of the wet material removed from test pit as follows:

$$m_{10} = m_8 - m_9 \quad (5)$$

where:

m_{10} = mass of wet material removed from test pit, kg,

m_8 = mass of wet material removed from test pit plus mass of container(s), kg, and

m_9 = mass of container(s) for m_8 , kg.

12.7 Calculate the wet density of the material removed from test pit as follows:

$$\rho_{wet} = \frac{m_{10}}{V_T} \times \frac{1}{10^3} \quad (6)$$



where:

ρ_{wet} = wet density of material excavated from test pit, Mg/m³,
 m_{10} = mass of wet material removed from test pit, kg, and
 V_T = volume of test pit, m³.

12.8 Calculate the dry density of the material removed from test pit as follows:

$$\rho_d = \frac{\rho_{wet}}{1 + \left(\frac{w}{100}\right)} \quad (7)$$

where:

ρ_d = dry density of material from test pit, Mg/m³,
 ρ_{wet} = wet density of material excavated from test pit, Mg/m³, and
 w = water content of material excavated from test pit, %.

13. Test Method B, Calculation

13.1 Calculate the wet mass of the oversize particles as follows:

$$m_{13} = m_{11} - m_{12} \quad (8)$$

where:

m_{13} = wet mass of oversize particles, kg,
 m_{11} = wet mass of oversize particles and container, kg, and
 m_{12} = mass of container, kg.

13.2 Calculate the wet mass of the control fraction as follows:

$$m_{18} = m_{10} - m_{13} \quad (9)$$

where:

m_{18} = wet mass of control fraction, kg,
 m_{10} = mass of wet material removed from test pit, kg, and
 m_{13} = wet mass of oversize particles, kg.

13.3 Calculate the volume of the oversize particles based on the mass in air and mass in water method as follows:

$$V_{os} = \frac{m_{13} - m_{14}}{1 \text{ g/cm}^3} \times \frac{1}{10^3} \quad (10)$$

where:

1 g/cm³ = density of water,
 $1/10^3$ = constant to convert g/cm³ to kg/m³,
 m_{13} = wet mass of oversize particles, kg, and
 m_{14} = mass of oversize particles suspended in water, kg.

13.4 Calculate the volume of the oversize particles based on a known bulk specific gravity as follows:

$$V_{os} = \frac{m_{13}}{G_m \times (1 \text{ g/cm}^3)} \times \frac{1}{10^3} \quad (11)$$

where:

V_{os} = volume of oversize particles, m³,
 m_{13} = wet mass of oversize particles, kg, and
 G_m = bulk specific gravity of oversize particles.

13.5 Calculate the volume of the control fraction as follows:

$$V_c = V_T - V_{os} \quad (12)$$

where:

V_c = volume of control fraction, m³,
 V_T = volume of test pit, m³, and
 V_{os} = volume of oversize particles, m³.

13.6 Calculate the wet density of the control fraction as follows:

$$\rho_{wet}(c) = \frac{m_{18}}{V_c} \quad (13)$$

where:

$\rho_{wet}(c)$ = wet density of control fraction, Mg/m³,
 m_{18} = wet mass of control fraction, kg, and
 V_c = volume of control fraction, m³.

13.7 Calculate the dry density of the control fraction as follows:

$$\rho_d(c) = \frac{\rho_{wet}(c)}{1 + \left(\frac{w_f}{100}\right)} \quad (14)$$

where:

$\rho_d(c)$ = dry density of control fraction, Mg/m³,
 $\rho_{wet}(c)$ = wet density of control fraction, Mg/m³, and
 w_f = moisture content of control fraction, %.

13.8 If required, convert dry density in inch-pound units, to SI units, using Eq. 8.

13.9 Calculate the dry mass of the control fraction as follows:

$$m_{19} = \frac{m_{18}}{1 + \left(\frac{w_f}{100}\right)} \quad (15)$$

where:

m_{19} = dry mass of control fraction, kg,
 m_{18} = wet mass of control fraction, kg, and
 w_f = water content of control fraction, %.

13.10 Calculate the dry mass of the oversize particles using one of the following equations as appropriate:

$$m_{17} = m_{15} - m_{16} \quad (16)$$

$$m_{17} = \frac{m_{13}}{1 + \left(\frac{w_{os}}{100}\right)} \quad (17)$$

where:

m_{17} = dry mass of oversize particles, kg,
 m_{15} = dry mass of oversize particles and container, kg,
 m_{16} = mass of container, kg,
 m_{13} = wet mass of oversize particles, kg, and
 w_{os} = water content of oversize particles, %.

13.11 Calculate the dry mass of the total sample as follows:

$$m_{20} = m_{19} + m_{17} \quad (18)$$

where:

m_{20} = dry mass of total sample (control fraction plus oversize), kg,
 m_{19} = dry mass of control fraction, kg, and
 m_{17} = dry mass of oversize particles, kg.



13.12 Calculate the percent oversize particles as follows:

$$p = \frac{m_{17}}{m_{20}} \times 100 \quad (19)$$

where:

p = percent oversize,
 m_{17} = dry mass of oversize particles, kg, and
 m_{20} = dry mass of total sample (control fraction plus oversize), kg.

13.13 Calculate the moisture content of the total material as follows:

$$w = \frac{m_{10} - m_{20}}{m_{20}} \times 100 \quad (20)$$

where:

w = moisture content of material excavated from test pit, %,
 m_{10} = mass of wet material removed from test pit, kg, and
 m_{20} = dry mass of total sample (control fraction plus oversize particles), kg.

13.14 It may be desired to express the results of the in-place density test as a Percent Compaction (D653), which is the ratio of the in-place dry density to the laboratory maximum dry density. The laboratory maximum dry densities are determined in accordance with Test Method D698, D1557, D4253, D4254, or D7382. Percent Compaction of the control fraction can be directly computed if Method B is used with restrictions (see Section 6). Calculations for determining relative density are provided in Test Method D4254. Corrections for oversize material, if required, should be performed in accordance with Practice D4718.

14. Report

14.1 The methodology used to specify how data are recorded is covered in 1.8.

14.2 Record as a minimum the following general information (data):

- 14.2.1 Project and Feature information,
- 14.2.2 Date of testing and personnel performing the test,
- 14.2.3 Test Location including coordinates or stationing, and elevation,
- 14.2.4 Site conditions that may influence the test, including surface conditions and weather conditions,
- 14.2.5 Visual description of the material, and
- 14.2.6 Comments on conduct of the test including any test conditions or difficulties affecting test results. Examples may include cobbles and boulders with angular edges and method of treatment, large inclusions left in the excavation, movement of

the frame, irregular voids, or deformation of the excavation. Photographs of the test are helpful to document conditions but not required to be reported.

14.3 Record as a minimum the following apparatus information:

14.3.1 Apparatus and methods for placing sand using the sand pouring device including density calibration data.

14.3.2 Apparatus and methods for determining the mass of soil excavated including scales used and their readability,

14.3.3 Apparatus and methods for determining the water content(s), of the total or control and oversize fractions, or both including ovens and scales, and,

14.3.4 Apparatus and methods for processing and weighing and determining the bulk specific gravity oversize particles, if required.

14.4 Record as a minimum the following test data/results:

14.4.1 Test hole volume to a minimum of four significant digits,

14.4.2 In-place wet density, total, or control fraction, or both, to three significant digits,

14.4.3 In-place dry density, total, or control fraction, or both, to three significant digits.

14.4.4 In-place water content(s), and total, or control fraction, or both, and test method(s) used, to three significant digits, and,

14.4.5 Bulk specific gravity and percentage of oversize particles to three significant digits.

15. Precision and Bias

15.1 *Precision*—Test data on precision is not presented due to the nature of the soil and rock materials being tested by these test methods. It is not feasible at this time to have ten or more agencies participate in an in situ testing program at a given site. Also, it is not feasible to produce multiple test locations having uniform properties. Any variation observed in the data is just as likely to be due to specimen variation as operator or laboratory testing variation.

15.1.1 Subcommittee D 18.08 is seeking any data from users of these test methods that might be used to make a limited statement on precision.

15.2 *Bias*—There is not accepted reference value for these test methods, therefore, bias cannot be determined.

16. Keywords

16.1 acceptance test; degree of compaction; density tests; field test; in-place density; pit test; quality control; sand replacement method



ANNEXES

(Mandatory Information)

A1. CALIBRATING SAND POURING EQUIPMENT AND SAND

A1.1 Scope

A1.1.1 This annex describes the procedure for calibrating sand pouring equipment and sand.

A1.1.2 The calibration determines an average density of poured sand for use in calculating the volume of a test pit excavated to determine in-place density of soil and rock.

A1.2 Summary of Test Method

A1.2.1 Using a specific pouring device, sand is poured into a calibration mold of similar size and shape of a field test pit to determine the density of the sand as poured under specific conditions.

A1.3 Significance and Use

A1.3.1 This calibration procedure is performed to obtain the value of density of the sand using a specific pouring device for use in measuring the volume of a field density test pit.

A1.3.2 This procedure should be performed:

A1.3.2.1 When a new supply of sand is processed into the storage bin.

A1.3.2.2 At intervals not exceeding 14 days when several unit weight tests are required on a daily basis.

A1.3.2.3 If tests are made at infrequent intervals, the sand must be calibrated before a test or series of tests is begun.

A1.3.2.4 For any change in equipment, personnel, or size or shape of the field test pit, (see 8.2.7 – 8.2.9).

A1.3.2.5 After any significant changes in atmospheric humidity, or change in moisture of the sand. The sand should be as dry as possible.

NOTE A1.1—Most sands have a tendency to absorb water from the atmosphere. A very small amount of absorbed moisture can make a substantial change in bulk density. In areas of high humidity or where the humidity changes often, the bulk density may need to be determined more often than the 14-day maximum interval indicated. The need for more frequent checks can be determined by comparing the results of different bulk-density tests on the same sand made in the area and conditions of use over a period of time.

A1.3.2.6 If tests are routinely made using reclaimed sand, calibrate when the cumulative mass of sand removed from the storage container equals the capacity of the container. A record of the mass of sand removed should be kept at a convenient location on or near the container.

A1.4 Apparatus

A1.4.1 *Metal Straightedge*—About 50 mm (2 in.) high, at least 3 mm ($\frac{1}{8}$ in.) thick, and with a length 1.5 times the side length of the calibration mold.

A1.4.2 *Mold*—A mold or container is required that is similar to the size and shape of the test pit excavated in the material. The volume of the mold shall be determined in accordance with the principles described in Test Method D4253.

A1.4.3 *Miscellaneous Equipment*—Buckets to mix and reclaim sand, pans, thick paper, and miscellaneous brushes and scoops for reclaiming sand.

A1.5 Technical Hazards

A1.5.1 Consistent sand flow (see 8.2.7 – 8.2.9).

A1.5.2 *Vibration of Poured Sand*:

A1.5.2.1 Any surface vibration or jarring of poured sand in the mold, whether the pouring process is complete or not, causes densification of the sand and results in erroneous test results. To achieve consistent results, the sand must be free to flow without any outside agitation.

A1.5.2.2 Striking off material above the top of the calibration mold must be done consistently with as little vibration as possible.

A1.5.2.3 Place calibration molds on rigid, vibration free surfaces while performing the calibration.

A1.5.3 *Reclaimed Sand*:

A1.5.3.1 As a general rule, reclaiming sand is no longer desirable or economically feasible.

A1.5.3.2 If sand is reclaimed, after each recovery it must be screened over a sieve that would pass its original maximum particle size to eliminate clay balls or other foreign matter. Discard the sand after three usages.

A1.6 Conditioning

A1.6.1 Store the sand in covered bins or containers to maintain a uniformly dry condition. A 55-gal barrel with a valve near the bottom makes an excellent storage container. An internal heat source, such as a heat tape, may be necessary in storage containers in areas that experience significant changes in atmospheric moisture.

A1.6.2 When a new supply of sand is introduced into the storage bin and before each calibration, thoroughly mix the sand and blend. Calibration records must document new shipments of sand and dates that new sand is introduced into the current storage bin.

A1.7 Procedure

A1.7.1 Determine and record the mass of the mold.

A1.7.2 Place the calibration mold on a rigid surface.

A1.7.3 Using the pouring device, pour the sand into the calibration mold, slightly overfilling. Use a circular motion to keep the sand surface relatively level. Keep the end of the spout about 50 mm (2 in.) above the sand surface while pouring. A constant sand surcharge level in the container, sand drop distance and the avoidance of any vibration of the measure are critical to the achievement of consistent results (see A1.5.2).

A1.7.3.1 If the reservoir capacity is too small to fill the calibration mold with one pour, use two or more pours to fill

the mold. See 8.2.8 for the procedure to follow when more than one pour is necessary.

A1.7.4 Strike off the excess sand even with the top of the calibration mold using the metal straightedge (see A1.5.2.2).

A1.7.5 Determine the mass of the sand and calibration mold and record.

A1.7.6 Calculate the mass of sand in the calibration mold and record.

A1.7.7 Calculate the density of the sand and record.

A1.7.8 Repeat the procedure in A1.7.1 – A1.7.7 as a second trial.

A1.7.9 Determine the uniformity of the two values obtained by dividing either value by the other. If the value of the ratio is between 0.990 and 1.010, inclusive, average the two values and record the average density. If the value of the ratio falls outside the limits, go to A1.7.10.

A1.7.9.1 Compare the average density with previously determined values to see if it is consistent and reasonable. If it is not, go to A1.7.10.

A1.7.10 Check to see that all equipment is performing correctly, that all calibrations are correct, and that the procedures and techniques used are correct. If no problems are discovered, then repeat procedure. If the values are still inconsistent, go to A1.7.11.

A1.7.11 Thoroughly mix all the sand being represented by this calibration and repeat the procedure. If the values are still inconsistent, discard all the sand and repeat the procedure using fresh sand from the original supply.

A1.8 Calculation

A1.8.1 Calculate the density of the sand as follows (ft-lb units can also be used):

$$\rho_s = \frac{m}{V} \times \frac{1}{10^3} \quad (\text{A1.1})$$

where:

ρ_s = density of sand, Mg/m³,

m = mass of sand in calibration mold, kg, and

V = volume of calibration mold, m³.

A2. GUIDELINES FOR TEST HOLE OR TEST DIMENSIONS AND SELECTION OF EQUIPMENT

A2.1 This annex covers guidelines for selecting the excavation dimensions and the type of equipment to use based on the maximum particle size present in the material (or control fraction) being tested. These guidelines apply to both these test methods and to the companion Test Method D5030 for using water replacement to determine the volume of an excavated test pit. The guidelines are given in Table A2.1 and Table A2.2. (Inch-pound equivalents for these two tables are provided in Table A2.3.) The typical types of test pit excavation shapes are shown in Fig. A2.1.

A2.2 These guidelines are based on providing a representative sample of the material being tested and on practical working conditions. For a discussion of the shape and dimen-

TABLE A2.2 Test Apparatus and Minimum Excavation Volume^A

NOTE 1—More than 200 mm maximum particle size should be determined on a case-by-case basis.

Maximum Particle Size, mm ^B	Minimum Required Volume, m ³	Suggested Apparatus and Template Opening, m	Required Minimum Depth, mm ^C	Approximate Diameter of Excavated Hole, m
75	0.03	825-mm square frame	250	0.75
125	0.06	1-m square frame	300	1
200	0.23	1.5-m diameter ring	450	1.5

^A Test Pit Type C (see Fig. A2.1).

^B Maximum particle size present in total material or the maximum particle size of control fraction if the total in-place density is not of concern.

^C This depth is necessary to obtain the minimum required volume of material when using the suggested apparatus and template opening.

sions of the test pits and for the minimum volumes for the excavation, see Appendix X1 in Test Method D5030.

A2.3 The guidelines shown in Table A2.1 apply to test pit Types A and B (see Fig. A2.1). These test pits generally are for non-free draining materials or for cohesionless materials whose gradation and particle angularity will allow near-vertical side walls to be excavated.

A2.4 The guidelines shown in Table A2.2 apply to test pit Type C (see Fig. A2.1). This type of test pit can be excavated when Type A or B cannot. For this case, the slope of the side walls will be much flatter, approximately the angle of repose of the material.

A2.5 These guidelines are only applicable when the limitations stated in 1.5 and 1.6 for unstable or soft materials are

TABLE A2.1 Test Apparatus and Minimum Excavation Volume^A

NOTE 1—More than 450 mm maximum particle size should be determined on a case-by-case basis.

Maximum Particle Size, mm ^B	Minimum Required Volume, m ³	Suggested Apparatus and Template Opening, m	Required Minimum Depth, mm ^C
75	0.03	0.6 m square frame	300
125	0.06	0.75 m square frame	450
200	0.23	1.2 m diameter ring	600
300	0.76	1.8 m diameter ring	600
450	2.55	2.7 m diameter ring	900

^ATest Pit Types A and B (see Fig. A2.1).

^B Maximum particle size present in total material or the maximum particle size of control fraction if the total in-place density is not of concern.

^C This depth is necessary to obtain the minimum required volume of material when using the suggested apparatus and template opening.



TABLE A2.3 Inch-Foot Equivalents for Table A2.1 and Table A2.2

followed.

Millimeters	Inches
75	3
125	5
200	8
250	10
300	12
450	18
600	24
750	30
825	33
875	35
900	36
1000	40
1350	54
1550	62
Metres	Feet
1.2	4
1.8	6
9	2.7
Cubic Feet	Cubic Metres
1.0	0.03
2	0.06
8	0.23
27	0.76
90	2.55

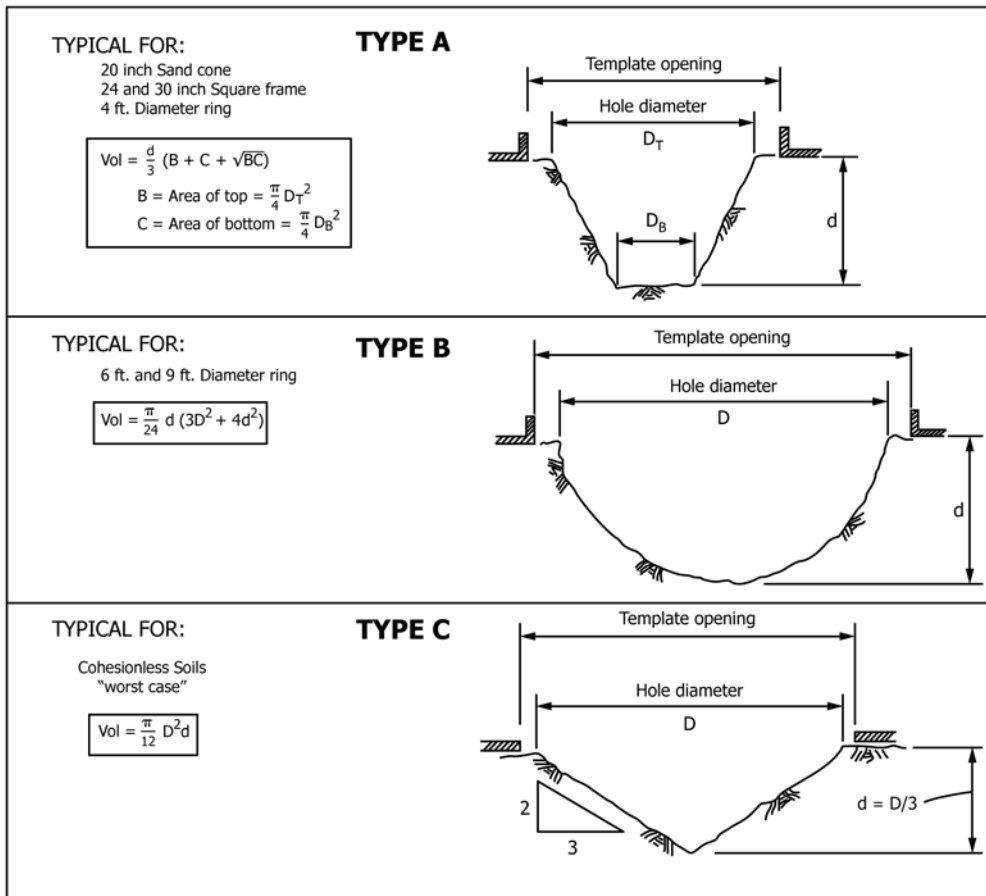


FIG. A2.1 Test Pit Configurations

APPENDIX

(Nonmandatory Information)

X1. EXAMPLE DATA FORM

X1.1 Example data form (Fig. X1.1) is taken from Earth Manual, Part II, Third Edition, Bureau of Reclamation, US

Department of the Interior, 1999, US GPO.



IN PLACE DENSITY TEST RECORD																				
SAMPLE NO. <i>Example</i>		FEATURE.		PROJECT																
TEST NO.		SOURCE OF MATERIAL																		
LOCATION		OFFSET		ELEV		ZONE														
TESTED BY	DATE	COMPUTED BY	DATE	CHECKED BY	DATE															
Cans 6, 7, 8, 9, 10, 11, 12 (1) Mass-Sand & Can(s). No(s). <u>350.00</u> lbm <u>50.00</u> lbm each (2) Mass-Sand Residue & Can(s) <u>87.51</u> lbm (3) Mass-Sand used. (1) (2) <u>262.49</u> l b . . . (4) Mass-Sand in Template ^(a) & Cone. No. <u>73.53</u> lbm (5) Mass-Sand in Hole. (3) (4) <u>188.96</u> lbm (6) Density of Calibrated Sand <u>98.1</u> lbm/ft ³ (7) Vol of Hole. $\frac{(5)}{(6)}$ <u>1.9262</u> ft ³		(22) Moisture Content. Oversize, w _{os} $\frac{(15)(21)}{(21)} \times 100$ <u>2.6</u> % (23) Mass-Wet Soil, (10) (15) <u>164.19</u> lbm (24) Wet Unit Weight of Soil, $\frac{(23)}{(17)}$ <u>143.9</u> lbf/ft ³ (25) Mass-Dry Soil, $\frac{(23)}{(w_f/100)}$ <u>146.34</u> lbm (26) Mass-Dry Soil & Oversize (25) + (21) <u>270.97</u> lbm (27) Percentage of Oversize, $\frac{(21)}{(26)} \times 100$ <u>46.0</u> % (28) Moisture Content, Soil & Oversize, W $\frac{(10)(26)}{(261)} \times 100$ <u>7.8</u> % (29) Dry Density Control Fraction $\frac{(24)}{1 + (w_f/100)}$ lbf/ft ³ <u>128.3</u> lbf/ft ³																		
(8) Mass-Wet Soil, Oversize & Can(s) <u>307.74</u> lbm (9) Mass-Can(s), No(s). <u>1, 2, 3</u> <u>15.68</u> lbm <u>5.23</u> , <u>5.20</u> , <u>5.25</u> (10) Mass-Wet Soil & Oversize (8) (9) <u>292.06</u> lbm (11) Wet Density Soil & Oversize $\frac{(10)}{(7)}$ <u>151.6</u> lbf/ft ³ (12) Dry Density Soil & Oversize. $\frac{(11)}{1 + (w_f/100)}$ lbf/ft ³ + <u>140.6</u> lbf/ft ³		<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="text-align: left;">Moisture Content Determination</th> <th style="text-align: left;">CONTROL FRACTION</th> </tr> </thead> <tbody> <tr> <td>(1) Mass-Wet Soil & Dish</td> <td style="text-align: center;">371.3 g</td> </tr> <tr> <td>(2) Mass Dry Soil & Dish</td> <td style="text-align: center;">346.2 g</td> </tr> <tr> <td>(3) Mass Dish No. <u>23</u></td> <td style="text-align: center;">140.2 g</td> </tr> <tr> <td>(4) Mass Water (1) (2)</td> <td style="text-align: center;">25.1 g</td> </tr> <tr> <td>(5) Mass Dry Soil (2) (3)</td> <td style="text-align: center;">206.0 g</td> </tr> <tr> <td>(6) Moisture Content $\frac{(4)}{(5)} \times 100$</td> <td style="text-align: center;">12.2 %</td> </tr> </tbody> </table>					Moisture Content Determination	CONTROL FRACTION	(1) Mass-Wet Soil & Dish	371.3 g	(2) Mass Dry Soil & Dish	346.2 g	(3) Mass Dish No. <u>23</u>	140.2 g	(4) Mass Water (1) (2)	25.1 g	(5) Mass Dry Soil (2) (3)	206.0 g	(6) Moisture Content $\frac{(4)}{(5)} \times 100$	12.2 %
Moisture Content Determination	CONTROL FRACTION																			
(1) Mass-Wet Soil & Dish	371.3 g																			
(2) Mass Dry Soil & Dish	346.2 g																			
(3) Mass Dish No. <u>23</u>	140.2 g																			
(4) Mass Water (1) (2)	25.1 g																			
(5) Mass Dry Soil (2) (3)	206.0 g																			
(6) Moisture Content $\frac{(4)}{(5)} \times 100$	12.2 %																			
(131) Mass-Wet Oversize ^(b) & Pan. <u>151.90</u> lbm (141) Mass Pan No. <u>24.03</u> lbm (15) Mass Wet Oversize ^(b) (13) (14) <u>127.87</u> lbm (16) Mass Oversize in Water lbm (17) Volume of Oversize ^(b) $\frac{(15)(16)^*}{261 \times 62.4}$ <u>0.7851</u> ft ³ (18) Sp. G. of Oversize ^(b) $\frac{(15)}{(16)}$ <u>2.6</u> [assumed <u>(16)</u>] (19) Mass-Dry Oversize & Pan <u>148.66</u> lbm (20) Mass-Pan. No. <u>13.24.03</u> lbm (21) Mass-Oven Dry Oversize (19) (20) <u>124.63</u> lbm		Soil Classification <u>GC</u> REMARKS <u>6' max. size</u> AUXILIARY TESTS 1435 <u>—</u> 1436 <u>89</u> 5300 <u>89</u> 5320 <u>89</u> 5505 <u>—</u>																		

* Or (17)_A by measuring the water displaced from a siphon can, then,
 (18)_A = $\frac{(15)}{(17) \times 62.4}$

(a) Template Calibration
 (1) Mass-Sand & Can(s) No. 4,5 100.00 lbm
 (2) Mass-Sand Residue & Can(s): 26.47 lbm
 (3) Mass-Sand in Template (1) (2) 73.53 lbm
 (b) Surface dried condition

FIG. X1.1 Example Data Form



SUMMARY OF CHANGES

Committee D18 has identified the location of selected changes to this standard since the last issue (D4914 – 08) that may impact the use of this standard. (March 1, 2016)

- | | |
|--|---|
| <p>(1) The standard was converted to SI metric with rationalized in-lb units.</p> <p>(2) Computation of Unit Weight was removed.</p> | <p>(3) The report section was revised to include information on significant digits.</p> |
|--|---|

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>