
**Nanotechnologies — Characterization of
volatile components in single-wall carbon
nanotube samples using evolved gas
analysis/gas chromatograph-mass
spectrometry**

*Nanotechnologies — Caractérisation des composants volatiles dans les
nanotubes de carbone à paroi simple (SWCNT) utilisant l'analyse des
gaz émis par chromatographie en phase gazeuse/spectrométrie de
masse*



Reference number
ISO/TS 11251:2010(E)

© ISO 2010

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO 2010

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	2
5 Apparatus	2
6 Sample preparation	3
7 Measurement procedures for EGA/MS and EGA/GCMS	3
7.1 General	3
7.2 Measurement procedure of EGA/MS	3
7.3 Measurement procedure of EGA/GCMS	4
8 Data analysis and interpretations of results	4
8.1 Qualitative analysis	4
8.2 Mass loss analysis	4
9 Precision and uncertainties	5
10 Test report	5
Annex A (informative) Case study	6
Bibliography	10

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

In other circumstances, particularly when there is an urgent market requirement for such documents, a technical committee may decide to publish other types of document:

- an ISO Publicly Available Specification (ISO/PAS) represents an agreement between technical experts in an ISO working group and is accepted for publication if it is approved by more than 50 % of the members of the parent committee casting a vote;
- an ISO Technical Specification (ISO/TS) represents an agreement between the members of a technical committee and is accepted for publication if it is approved by 2/3 of the members of the committee casting a vote.

An ISO/PAS or ISO/TS is reviewed after three years in order to decide whether it will be confirmed for a further three years, revised to become an International Standard, or withdrawn. If the ISO/PAS or ISO/TS is confirmed, it is reviewed again after a further three years, at which time it must either be transformed into an International Standard or be withdrawn.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO/TS 11251 was prepared by Technical Committee ISO/TC 229, *Nanotechnologies*.

Nanotechnologies — Characterization of volatile components in single-wall carbon nanotube samples using evolved gas analysis/gas chromatograph-mass spectrometry

1 Scope

This Technical Specification specifies a method for the characterization of volatile components in single-wall carbon nanotubes (SWCNTs) samples using evolved gas analysis/gas chromatograph mass spectrometry (EGA/GCMS).

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO/TS 27687, *Nanotechnologies — Terminology and definitions for nano-objects — Nanoparticle, nanofibre and nanoplate*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO/TS 27687 and the following apply.

3.1

evolved gas analysis

EGA

technique in which the nature and/or amount of volatile product(s) released by a substance subjected to a controlled temperature program is(are) determined

NOTE The method of analysis should always be clearly stated (Reference [1] in the Bibliography).

3.2

evolved gas analysis/mass spectrometry

EGA/MS

technique using mass spectrometry to analyse gaseous components evolved from a sample as a function of temperature

NOTE Although the gases evolved at any particular temperature are detected simultaneously, it might not be possible to uniquely identify the different components using MS alone.

3.3

evolved gas analysis/gas chromatograph mass spectrometry

EGA/GCMS

technique combining a gas chromatograph and a mass spectrometer to identify the chemical composition of gases evolved from a sample as a function of temperature

NOTE The evolved gases are passed through a gas chromatograph (GC) to separate each component so that it can be identified in the MS unit.

3.4

volatile compounds

compounds that are evolved from a sample at the temperature under consideration

4 Principle


EGA/MS and EGA/GCMS are used to characterize volatile impurities in samples of SWCNT. Volatile compounds are identified by measuring the mass spectra of the gaseous component evolved from the heated samples in a furnace or other suitable heating device, such as that used for programmed temperature pyrolysis or thermogravimetric analysis. EGA/MS is used to determine the temperature range over which the release of volatile components occurs. EGA/GCMS analysis is used to identify each component separately by the use of a capillary column. Quantitative information can additionally be obtained by the sample mass loss in thermogravimetric analysis (TGA) and the peak area in EGA/MS.

NOTE Some details of the technique are described in References [2] to [6] in the Bibliography. EGA/GCMS plays a complementary role to TGA, which is mainly devoted to quantifying the mass of the volatile components.

5 Apparatus


Figure 1 shows a schematic diagram of EGA/MS which is composed of a furnace, a heating unit without a separation column and a MS unit. In the EGA/MS, evolved gas from the furnace is led to the MS unit directly through a capillary tube without a separation process.

Figure 2 shows a schematic diagram of an EGA/GCMS which is composed of a furnace, a GC with a separation column and an MS unit. In the EGA/GCMS, all compounds evolved from the sample within the furnace are captured by the cooling trap and are then introduced to the GC unit by heating the trap. The compounds are separated by the column in the GC unit.

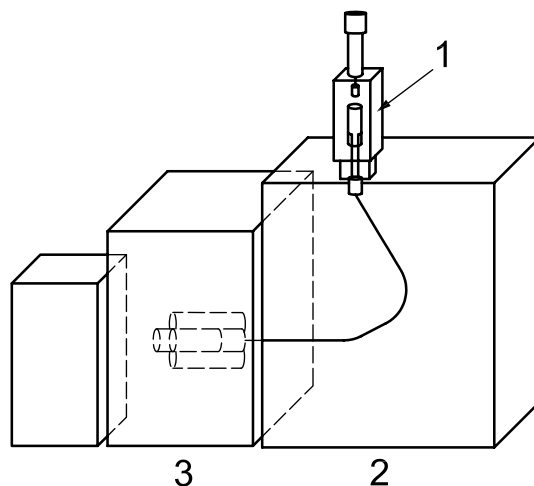**Key**

- 1 furnace
- 2 heating unit
- 3 MS unit

Figure 1 — Schematic diagram of EGA/MS

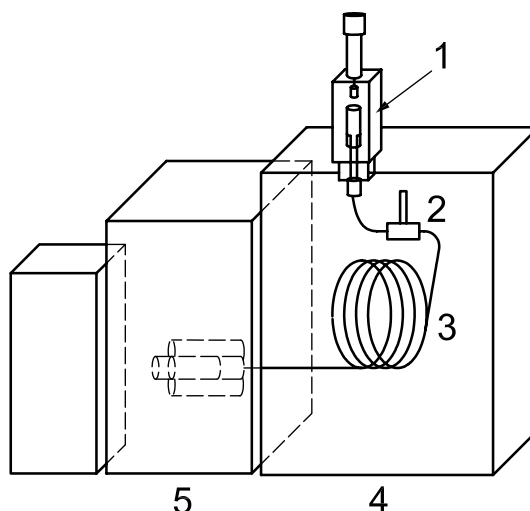

Key

- 1 furnace
- 2 cooling trap
- 3 capillary column
- 4 GC unit
- 5 MS unit

Figure 2 — Schematic diagram of EGA/GCMS

6 Sample preparation

Sample preparation, such as dissolution or dispersion, is not required. For a qualitative analysis, the sample shall be introduced into the EGA/MS or EGA/GCMS as it is. In order to avoid the vaporization of any volatiles that might be present, samples shall not be dried before analysis.

7 Measurement procedures for EGA/MS and EGA/GCMS

7.1 General

Load the SWCNT sample into the furnace and heat it up to identify the temperature range of gasification using EGA/MS measurement, and use the EGA/GCMS to identify each component at the designated temperature range.

7.2 Measurement procedure of EGA/MS

Weigh between 0,5 mg and 2 mg of the SWCNT sample, to the nearest 0,01 mg, using a calibrated mass balance.

Load the weighed sample into the furnace, including the sample cup used when weighing.

Heat the sample at a constant rate until gas evolution stops. Measure the total ions from volatile components. Determine the start temperature and the end-point of gasification using the EGA curve.

Compare the observed MS spectrum with the MS spectral database and determine each component in the evolved gas species. For appropriate comparison of MS spectra, an ionization voltage shall be in accordance with the voltage of the spectral database.

Perform EGA/GCMS if the measured spectrum cannot be identified using the MS spectral database due to its mixed components (see 7.3).

Weigh the sample after EGA/MS measurement, to the nearest 0,01 mg.

NOTE The rate of heating depends on the calorific capacity of the sample. Generally a range of 15 to 25 °C/min is used for EGA/MS.

7.3 Measurement procedure of EGA/GCMS

Weigh between 0,5 mg and 2 mg of SWCNT from the same sample as that used in 7.2, to the nearest 0,01 mg.

Load the sample into the furnace.

Heat up the sample at a constant rate to the lower temperature of either the end-point of the gasification or upper limit of the instrument.

Compare the observed MS spectrum with the mass spectral database and determine each component of the evolved gas species. An ionization voltage shall be in accordance with the voltage of the standard spectra.

The MS detector shall be calibrated by using a calibration reference material.

NOTE The rate of heating depends on the sample. Generally, a range of 45 to 65 °C/min is used for EGA/GCMS to shorten the analytical time.

8 Data analysis and interpretations of results

8.1 Qualitative analysis

The qualitative analysis shall be based upon the standard spectral information of compounds. Components from evolved gas shall be determined by comparing the measured MS spectra with a mass spectral database.

- a) Choose the component that needs to be identified.
- b) Subtract the background from the targeted MS spectrum.
- c) Search for similar spectra from within the spectral database.
- d) Select the probable components in the sample from the candidates identified using the standard spectra.

NOTE 1 Many kinds of software for searching and a mass spectral database are available, as an example, NIST/EPA/NIH Mass Spectral Library with Search Program.

NOTE 2 Using this method, *n*-hexane, benzene and toluene were identified in the example shown in Annex A and Figure A.4.

8.2 Mass loss analysis

The volatile components in SWCNT samples are determined using the following formula:

$$P = \frac{W_0 - W_t}{W_0} \times 100$$

where

P is the volatile impurity content, expressed as a percentage;

W_0 is the sample mass, in milligrams, before heating;

W_t is the sample mass, in milligrams, after heating.

NOTE Normally, quantitative analysis by GC/MS needs calibration curves, which show the relationship of the signal intensity and the concentration of each component. It is impossible to prepare the calibration curves for all components of interest. For this reason, only mass loss by the EGA process is used.

9 Precision and uncertainties

Currently, the uncertainties in the volatile components characterizations for SWCNTs by EGA/GCMS comes from

- a) fluctuation of temperature in the oven or detector,
- b) mis-calibration of the MS detector, or
- c) fluctuation of ionization voltage.

10 Test report

The test report shall include the following information:

- a) a reference to this Technical Specification;
- b) identified components;
- c) mass loss in percentage (%);
- d) heating conditions.

Annex A (informative)

Case study

A.1 General

An example of different analytical conditions is given in A.2.

A.2 Measurement parameters

The measurement parameters are as follows:

a) EGA/MS

EGA unit

Furnace temperature	1) Hold sample at 40 °C for 2 min. 2) Heat sample from 40 °C to 750 °C at 20 °C/min.
---------------------	---

GC (Oven)

Column	Deactivated capillary tube [2,5 m × 0,15 mm internal diameter (ID)]
Column temperature	300 °C (maintained temperature of GC oven)
Carrier gas	Helium (99,99 %)
Column head pressure	60 kPa
Injection temperature	230 °C
Injection method	Split 1:15

MS

Ion-source temperature	200 °C
Interface temperature	300 °C
Ionization method	Electron ionization
Ionization energy	70 eV
Scan range	mass-to-charge ratio (m/z) 10 to 400
Scan interval	5 s

b) EGA/GCMS

EGA unit

Furnace temperature	Heat sample from 150 °C to 600 °C at 60 °C/min
---------------------	--


GC

Column	GS-GasPro (30 m × 0,32 mm (ID))
Column temperature	40 °C (1 min hold) to 200 °C at 40 °C/min to 250 °C at 25 °C/min, 250 °C (23 min hold)
Carrier gas	Helium (99,99 %)
Column head pressure	60 kPa
Injection temperature	230 °C
Injection method	Split 1:15

MS

Ion-source temperature	200 °C
Interface temperature	260 °C
Ionization method	Electron ionization
Ionization energy	70 eV
Scan range	m/z 10 to 400
Scan interval	0,5 s

An EGA chromatogram from EGA/MS is shown in Figure A.1. For this SWCNT sample, the main evolved component was observed between 200 and 600 °C. In this evolved gas profile, the m/z of water, oxygen and nitrogen were subtracted to reduce influences.

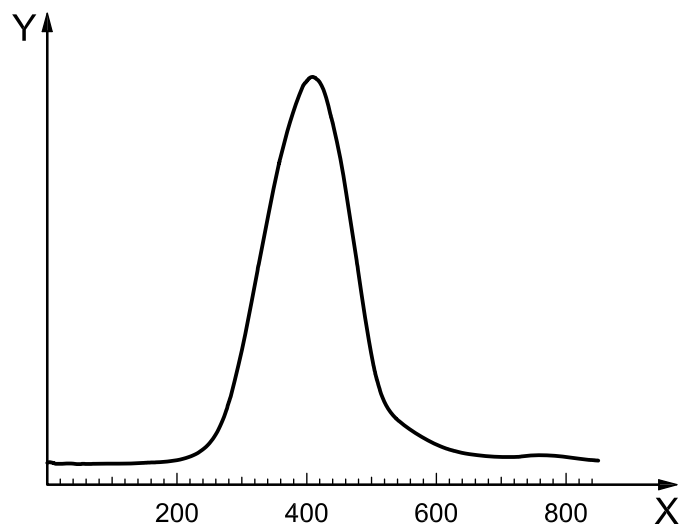


Key

X temperature, °C
Y abundance

Figure A.1 — Evolved gas profile by EGA/MS

Based on the result of the evolved gas profile, EGA/GCMS analysis was conducted to identify the volatile components. The total ion chromatogram (TIC) from the EGA/GCMS is shown in Figure A.2. The TIC is the chromatogram obtained by plotting the total electron current emitted from fragments as a function of the retention time.

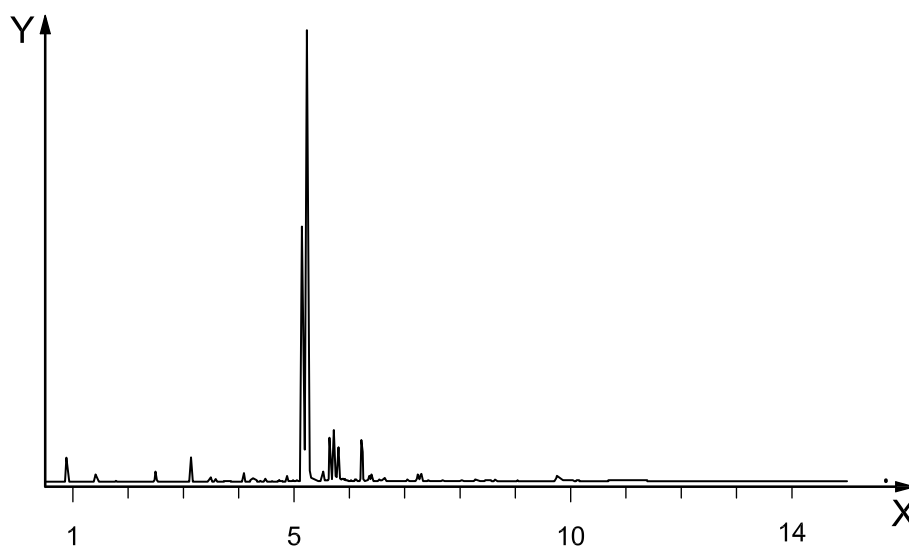


Key


X retention time, min
Y abundance

Figure A.2 — Total ion chromatogram of EGA/GCMS

By analysing the MS spectra of the peaks from this chromatogram, identification of each component was made. Several peaks were observed on the TIC. Figure A.3 shows a MS spectrum of the peak at about 5 min.

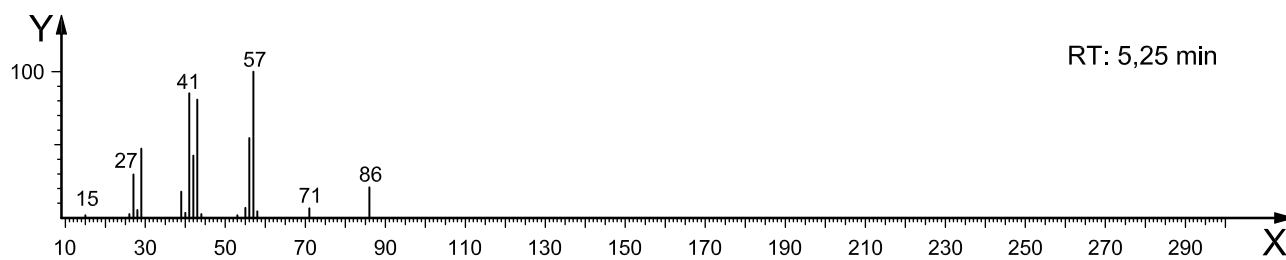

a) MS spectrum of the peak at about 5 min of retention time (RT)

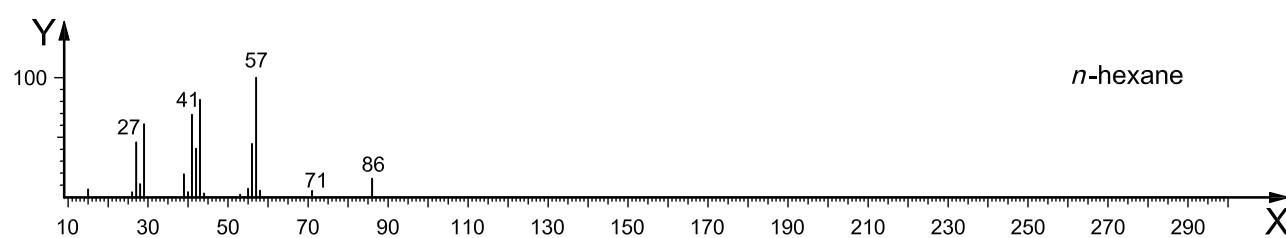


b) MS spectrum of *n*-hexane from standard library

Key

X *m/z*

Y relative abundance

Figure A.3 — Identification of MS spectrum

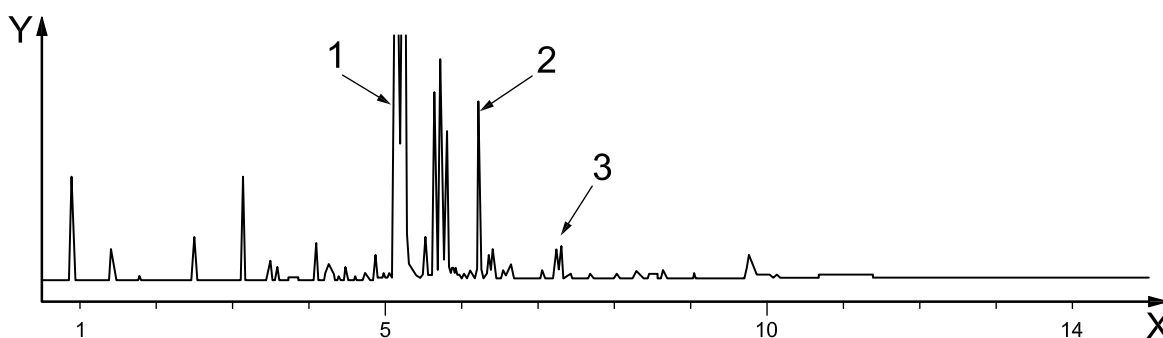

Key

1 *n*-hexane


2 benzene

3 toluene


Figure A.4 — Assignment of several components from a SWCNT sample

This compound was identified as *n*-hexane by comparison with reference spectra. By analysing the MS spectra, other peaks were assigned to benzene and toluene as shown in Figure A.4.


The mass reduction of the sample was approximately 0,055 mg from its original total mass 1,328 mg. This showed that 4 % of the total mass was due to volatile impurities including moisture in the SWCNTs.

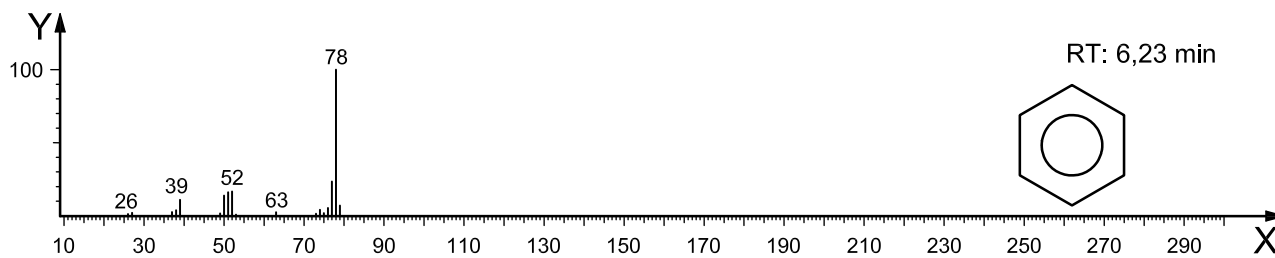


a) MS spectrum of the peak at about 6 min of RT in Figure A.2

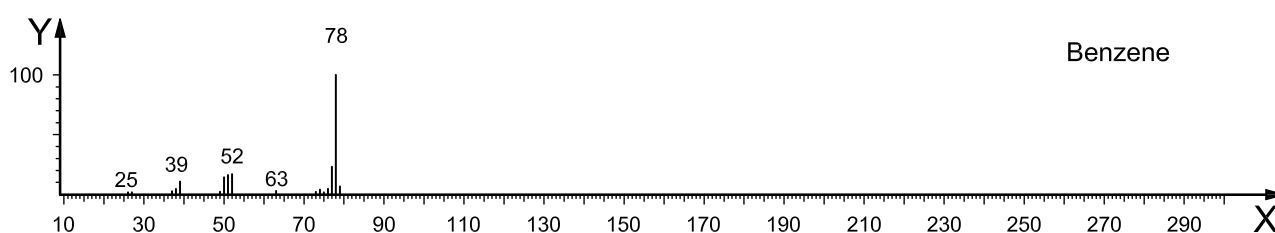

b) MS spectrum of benzene from standard library

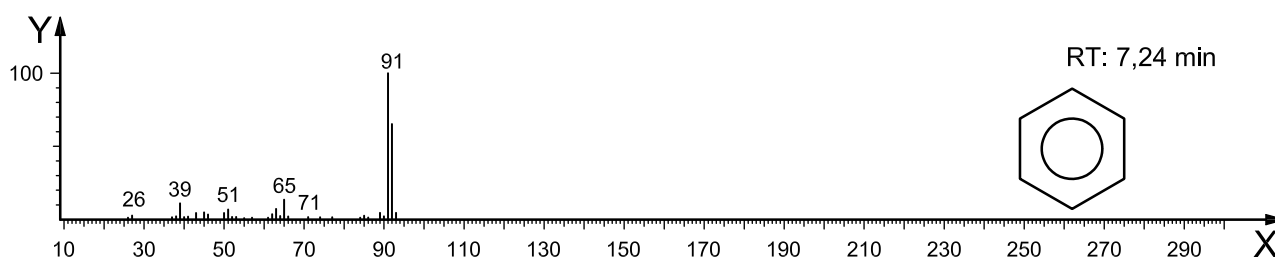

c) MS spectrum of the peak at about 7 min of RT in Figure A.2

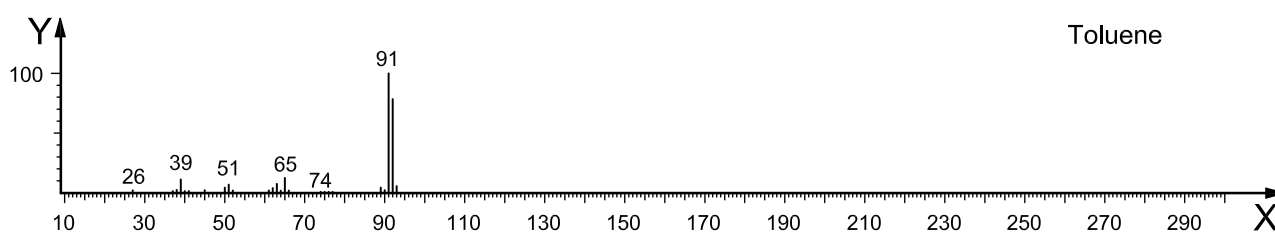

d) MS spectrum of toluene from standard library

Key

X m/z

Y relative abundance

Figure A.5 — MS spectra of the peak at about 6 and 7 min in Figure A.4 (upper) and MS spectra of benzene and toluene from standard spectral database (lower)

Bibliography

- [1] IUPAC Compendium of Chemical Terminology 2nd Edition (1997)
- [2] STEVENS, M. P.; *Characterization and Analysis of Polymers by Gas Chromatography*, (Marcel Dekker), New York (1969)
- [3] TSUGE, S.; Structural Characterization of Polymers by Pyrolysis-Gas Chromatography. *Trends Anal. Chem.*, 1981, **1**, pp. 87-90
- [4] TSUGE, S and OHTANI, H.; Structural Characterization of Polymeric Materials by Pyrolysis-GC/MS, *Plym. Degrad. and Stab.*, 1997, **58**, pp. 109-130
- [5] MOLDOVEANU, S. C.; Pyrolysis GC/MS, Present and Future (Recent Past and Present Needs), *J. Microco. Sep.*, 2001, **13**, pp. 102-125
- [6] TSUGE, S and OHTANI, H.; WATANABE, C. and KAWAHARA, Y; Application of a Multifunctional Pyrolyzer for Evolved Gas Analysis and Pyrolysis-GC of Various Synthetic and Natural Materials, *Am. Lab.*, 2003, **35(1)**, pp. 32-37

